

**Draft** Report of Investigations 96XX

## **Laboratory and Field Performance of a Respirable Personal Dust Monitor**

**By Jon C. Volkwein, Robert P. Vinson, Steven J. Page, Linda J. McWilliams,  
Gerald J. Joy, Steven E. Mischler, and Donald P. Tuchman**

**This draft publication has been released for public viewing and  
comments before final publication. Comments may be sent to  
[pdmcomments@cdc.gov](mailto:pdmcomments@cdc.gov) or in writing to the authors at NIOSH,  
P.O. Box 18070, Pittsburgh, PA 15236.**

### **DEPARTMENT OF HEALTH AND HUMAN SERVICES**

Centers for Disease Control and Prevention  
National Institute for Occupational Safety and Health  
Pittsburgh Research Laboratory  
Pittsburgh, PA

May 2006

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

Disclaimer: Mention of any company or product does not constitute endorsement by the National Institute for Occupational Safety and Health (NIOSH). In addition, citations to Web sites external to NIOSH do not constitute NIOSH endorsement of the sponsoring organizations or their programs or products. Furthermore, NIOSH is not responsible for the content of these Web sites.

**DHHS (NIOSH) Publication No. 2006–XXX**

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

# CONTENTS

	<i>Page</i>
Abstract.....	7
Introduction .....	8
Description of the PDM.....	9
System configuration.....	10
Sample flow path.....	11
Flow measurement and control.....	12
Battery configuration.....	12
Data treatment.....	13
TEOM mass measurement technique .....	13
Momentum compensation: the key to miniaturization .....	14
Methods .....	14
Laboratory methods.....	14
Dust exposure chamber .....	14
Samplers .....	15
PDM .....	15
Gravimetric reference .....	16
Impactors.....	16
Analytical gravimetric precision .....	16
Experimental design.....	17
PDM battery test.....	18
PDM mass constant verification.....	18
Definition of constant.....	19
Procedure to determine mass constant.....	19
Analysis .....	20
Detailed in-mine test methods .....	21
Criteria for mine selection.....	21
Detailed mine procedures.....	21
Area sampling .....	22
Maintenance and use log .....	23
Field precision analysis .....	23
Results .....	24
Laboratory accuracy verification .....	24
Premine testing.....	24
Postmine testing .....	25
Accuracy .....	26
Calibration constant $K_0$ .....	27
Limit of detection and quantification .....	28
Battery depletion effects.....	29
Detailed in-mine testing.....	30
Performance over project duration.....	30
Extended testing .....	31
Maintenance results.....	31
Underground precision.....	33
Discussion.....	34
Training and comments .....	34
Screen presentation of data.....	35
Performance issues .....	36
Data files.....	37
Download .....	37
Interpretation.....	39

Error codes.....	39
Meaning and interpretation.....	39
Distinguishing valid data .....	40
Instrument bias sources.....	41
Maintenance.....	42
Calibration .....	42
Flow.....	42
Mass.....	43
Precision .....	44
Conclusion.....	44
Acknowledgments.....	45
References .....	46
Appendix A.—Detailed mine PDM concentration data .....	48
Appendix B.—Detailed mine Lippmann sampler data.....	50
Appendix C.—Analysis of voided respirable coal mine dust samples collected, 1995–2004.....	52

## ILLUSTRATIONS

1. PDM internal components .....	10
2. Precommercial PDM connected to docking station used for charging and communication with a PC using an RS–232 interface .....	11
3. Technician changing filter on the PDM mass sensor.....	12
4. Laboratory test chamber and arrangement of instruments .....	17
5. Battery testing to failure using flow rate as an indicator .....	29
6. Basic PDM screen display formats and information presented .....	35
7. Example of data printout .....	38
8. Detail of results from sample shown in figure 7 .....	39
9. Mass offset "error" resulting from pinched tube and subsequent recovery of correct mass measurements.....	41

## TABLES

1. Detailed mine characteristics and location of Lippmann sample.....	21
2. Premine laboratory data of reference mass measurements and PDM mass measurements .....	25
3. Postmine laboratory data of references mass measurements and PDM mass measurements .....	26
4. PDM pre- and postmine lab accuracy calculations .....	27
5. Comparison of PDM measured <i>K0</i> and programmed <i>K0</i> .....	28
6. Total samples taken during detailed mine sampling and number of valid samples when NIOSH was present or absent from the mine property.....	30
7. Summary of PDM use and repair by quintile .....	32
8. Overall success rate .....	33
9. Field precision results .....	34
10. PDM performance issues and comments .....	36
11. Flow calibration history .....	43
C–1. Analysis of voided respirable coal mine dust samples collected, 1995–2004.....	52

## ACRONYMS AND ABBREVIATIONS USED IN THIS REPORT

ANOVA	analysis of variance
BMRC	British Medical Research Council
CL	confidence limit
CMDPSU	coal mine dust personal sampler unit
DO	Dorr-Oliver
EOS	end of shift
GSD	geometric standard deviation
HD	Higgins-Dewell
HEPA	high-efficiency particulate air (filter)
ISO	International Organization for Standardization
LED	light-emitting diode
LOQ	limit of quantification
MMAD	mass median aerodynamic diameter
MO	mass offset
MRE	Mining Research Establishment (U.K.)
MSHA	Mine Safety and Health Administration
NIOSH	National Institute for Occupational Safety and Health
NIST	National Institute of Standards and Technology
PC	personal computer
PDM	personal dust monitor
PEL	permissible exposure limit
PVC	polyvinyl chloride
RH	relative humidity
RMSE	root mean square error
RSD	relative standard deviation
TE	tapered element
TEC	Thermo Electron Corp. (Albany, NY)
TEOM	tapered-element oscillating microbalance
UCL	upper confidence limit

**UNIT OF MEASURE ABBREVIATIONS USED IN THIS REPORT**

hr	hour
in	inch
kg	kilogram
L/min	liter per minute
lb	pound
mg	milligram
mg/m <sup>3</sup>	milligram per cubic meter
min	minute
mm	millimeter
mm Hg	millimeter of mercury
sec	second
μg	microgram
μm	micrometer
°C	degree Celsius
°F	degree Fahrenheit

## LABORATORY AND FIELD PERFORMANCE OF A RESPIRABLE PERSONAL DUST MONITOR

By Jon C. Volkwein,<sup>1</sup> Robert P. Vinson,<sup>2</sup> Steven J. Page,<sup>3</sup> Linda J. McWilliams,<sup>4</sup>  
Gerald J. Joy,<sup>5</sup> Steven E. Mischler,<sup>6</sup> and Donald P. Tuchman<sup>5</sup>

---

### ABSTRACT

The National Institute for Occupational Safety and Health (NIOSH), through an informal partnership with industry, labor, and the Mine Safety and Health Administration, has developed and tested a new type of instrument known as the personal dust monitor (PDM). The dust monitor is an integral part of the cap lamp that miners normally carry to work and provides continuous information about the amount of respirable coal mine dust in the breathing zone of that individual. Testing was conducted in the laboratory to verify the instrument's accuracy as received from the manufacturer and after a period of underground use of the instrument. In-mine testing determined the precision, durability, and miner acceptance. The laboratory testing verified previous work that there is a 95% confidence that the individual PDM measurements were within  $\pm 25\%$  of the reference measurements. The means of the pre- and postmine accuracy verification test values for 25 PDMs were statistically equivalent. Data from the mines showed a field precision of 0.078 relative standard deviation for the PDM and 0.052 for the coal mine dust personal sampler unit. The PDM had about 90% availability for collecting valid information in over 8,000 hr of underground use. Anecdotal comments by miners indicated that they found the PDM more convenient to wear for sampling than currently used instruments. Additional data were collected to measure the equivalency of the PDM to the U.K. Mining Research Establishment standard as required by U.S. law. However, analysis of the data was more complex than originally anticipated because the increasing variance with concentration required use of a more sophisticated statistical model. Explanation of and results from this work will be the subject of a future publication. Under the broad range of test conditions covered in this work, the PDM functioned as well as the current sampler in terms of availability for use, accuracy, precision, and miner acceptance.

---

<sup>1</sup>Research physical scientist.

<sup>2</sup>Physicist.

<sup>3</sup>Research physicist.

<sup>4</sup>Statistician.

<sup>5</sup>Industrial hygienist.

<sup>6</sup>Physical scientist.

Pittsburgh Research Laboratory, National Institute for Occupational Safety and Health, Pittsburgh, PA.

## INTRODUCTION

Measurement of workplace dust is an essential first step in eliminating lung disease caused by overexposure to dust. The Federal Coal Mine Health and Safety Act of 1969, the predecessor to the Federal Mine Safety and Health Act of 1977, mandates that coal mine dust levels be monitored and controlled to at or below  $2 \text{ mg/m}^3$  for a shift. To date, this monitoring process has relied upon a coal mine dust personal sampler unit (CMDPSU) to collect a filter sample in the mine environment. The filter is then sent to a laboratory for analysis and the results returned to the mine operators several days or occasionally weeks after the actual sample was taken. Following a long history of developmental efforts associated with light-scattering [Williams and Timko 1984], fixed-site, and personal continuous dust monitors [Kissell and Sacks 2002], the Secretary of Labor and the Federal Advisory Committee on the Elimination of Pneumoconiosis Among Coal Mine Workers [U.S. Department of Labor 1996] directed the National Institute for Occupational Safety and Health (NIOSH) to embark on research to improve sampling instrumentation for use in the mining industry. In consultation with labor, industry, and government, NIOSH issued a contract to Rupprecht and Patashnick Co., Inc. (now Thermo Electron Corp. (TEC)), Albany, NY, (CDC contract 200–98–8004) to develop a one-piece personal dust monitor (PDM). The PDM is based on an environmental ambient air monitor that has achieved global acceptance for use in air quality monitoring networks. The important aspect of this monitor is that it directly measures the mass of dust on a filter regardless of dust composition, size, or physical characteristics. This contract work successfully miniaturized the air quality monitor's sensor and incorporated the sensor into a prototype person-wearable dust monitor that provided accurate end-of-shift (EOS) data to miners [Volkwein et al. 2004]. Laboratory results from this work demonstrated that with different coal types and size distributions there was a 95% confidence that the individual PDM measurements were within  $\pm 25\%$  of the reference measurements. Mine test results comparing the PDM prototype with adjacent reference samplers indicated that the measurements were statistically indistinguishable. The technology proved durable enough to successfully measure 108 shifts of data out of 115 attempts in the mines. Under these specific test conditions, the PDM was shown to be convenient to wear and robust to use, provided accurate data, provided timely data that could be used to monitor and prevent overexposure, and was easy to use.

Encouraged by the promising results from the initial laboratory and in-mine tests of the prototype PDM, the Mine Safety and Health Administration (MSHA) announced in June 2003 that it would suspend all work to finalize the proposed dust rules published in March 2003 and pursue accelerated research on the PDM [MSHA 2003]. In addition, the other PDM development partners, consisting of labor and industry, contributed toward drafting a test protocol to determine if the PDM was in fact suitable for use in coal mines, was durable for everyday mine use, and ergonomically acceptable to miners. Another part of the protocol required measuring the precommercial PDM performance in the laboratory and in mine environments for accuracy, precision, functionality, and long-term performance.

This report includes the first two of three major areas studied. The first is a confirmation that the precommercial PDM's laboratory accuracy is similar to that of the prototype instrument and that the accuracy is maintained after use of the instrument in mines. The second area is a detailed



underground evaluation that includes measurement of the precision of the PDM, the CMDPSU, and the impactor to be used to measure the dust size distribution. The detailed underground evaluation also determines the performance of the PDM while in routine use by miners. The third area of this testing—to determine the equivalency of the PDM to standards of the U.K. Mining Research Establishment (MRE) and the International Organization for Standardization (ISO) for underground mines—is more complex than originally anticipated and will require use of a more sophisticated statistical model than originally planned. In order to proceed with the finished portion of this work, NIOSH has elected to present this work in a subsequent publication.

The fraction of dust that is considered respirable is an important part of measuring a worker's risk from dust. ISO [1995] has recommended that the definition of respirable dust follow the convention described by Soderholm [1989]. Because no device precisely follows this theoretical convention, specific size classification devices that are used exhibit inherent bias when attempting to duplicate the convention. In fact, the 10-mm Dorr-Oliver (DO) dust cyclone currently used in the CMDPSU has bias relative to both the ISO and the British Medical Research Council (BMRC) definition of respirable dust [Bartley et al. 1994]. The BMRC definition was adopted by MRE as the convention used to relate dust concentrations to worker health effects. The cyclone chosen for use in the PDM required a configuration that could accept the tube coming from the hard hat inlet. The cyclone selected followed the Higgins-Dewell (HD) design previously shown through testing to have low bias relative to the ISO convention [Maynard and Kenny 1995].

This report presents the theory of operation, description, performance of the PDM compared to gravimetric-based reference dust sampling methods, and functionality of the instrument when used by miners. We specifically address the accuracy of the instrument before and after mine testing and the in-mine precision.

## **DESCRIPTION OF THE PDM**

The dust monitor described in this report is a precommercial (not for general sale) Model 3600 PDM that functions identically to a prototype monitor originally developed under contract. This PDM differs from the prototype in that it incorporates a stronger case, improved display, more efficient power management, and improved software. The device is intended to be virtually “invisible” to the miner as a replacement for the cap lamp and battery currently used in mines.

The tapered-element oscillating microbalance (TEOM) mass sensor was the key to the accurate, time-resolved measurements provided by the PDM [Patashnick and Rupprecht 1991]. TEC has applied this mass measurement technique in a variety of arenas requiring time-resolved measurements, including ambient air, diesel, and stack particulate monitoring. This inertial, gravimetric-equivalent, mass measurement technique typically provides a limit of detection equivalent to that of the most sensitive laboratory-based microbalances. The development of the TEOM technique for use in a small personal exposure monitor subjected to the harsh conditions of an underground mine brought new challenges. As a result of a multiyear effort, TEC invented a hardware-based momentum compensation approach that effectively isolated the mass monitor

from external shocks and was essential to providing microgram mass resolution in challenging applications.

### System Configuration

The PDM is a respirable dust sampler and cap lamp configured to have dimensions and weight similar to those of a current lead-acid-type miner's cap lamp battery. Components of the device include a sample inlet tube, HD cyclone, air heater, pump, dust sensor, battery for the sampler, battery for the cap light, electronic control and memory boards, a display screen, and Windows®-based computer interface software called WinPDM. Figure 1 shows some of these components. The enclosure of the PDM is hardened to withstand the harsh conditions found in the mine environment, with the system designed to meet MSHA drop test requirements for cap lamps (30 CFR<sup>7</sup> 19) as well as intrinsic safety-type approval requirements (30 CFR 18). The PDM system also includes a nonintrinsically safe docking station simultaneously used to communicate with PC software for programming and retrieving stored data in the instrument and to recharge its batteries for the next work shift (Figure 2).

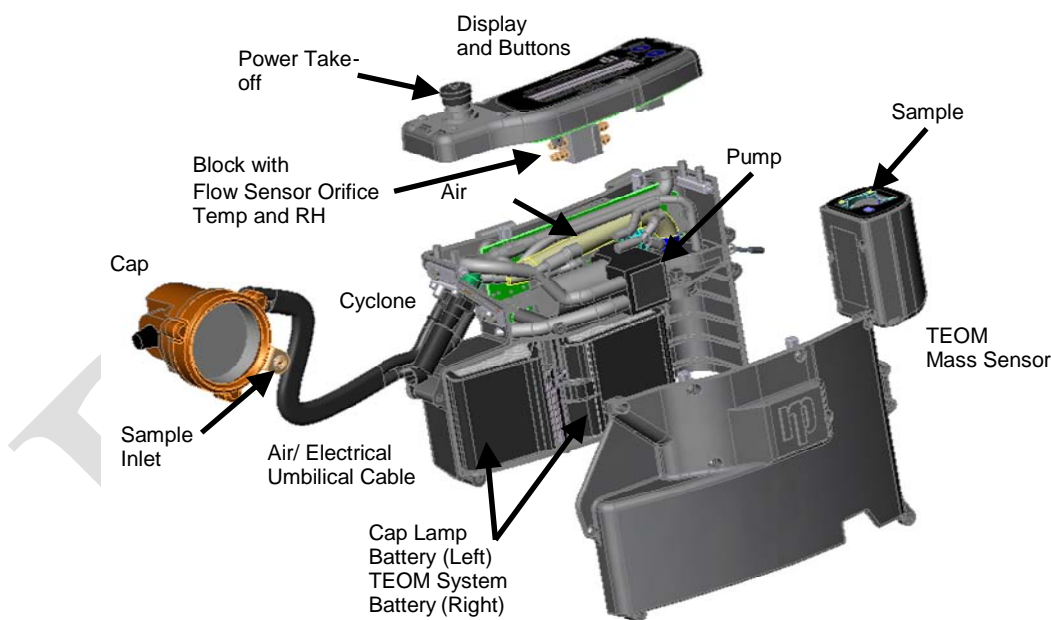


Figure 1.—PDM internal components.

<sup>7</sup>Code of Federal Regulations. See CFR in references.



**Figure 2.—Precommercial PDM connected to docking station used for charging and communication with a PC using an RS-232 interface.**

### **Sample Flow Path**

A 2.2 L/min flow of particle-laden air from the mine atmosphere enters an inlet mounted adjacent to the cap lamp mounted on the bill of the miner's hard hat and passes through flexible conductive tubing before reaching the HD cyclone at the entrance of the PDM. The cyclone separates the dust and allows particles that could penetrate to the lung—respirable dust—to proceed through a heated section of tubing to remove excess moisture and then to enter the unit's mass sensor. As the airflow passes through the mass sensor, an exchangeable filter cartridge collects the respirable particles. The mass sensor can be removed from the PDM by a mine's dust technician (Figure 3) to change the particle collection filter and clean the unit after the end of each work shift.



**Figure 3.—Technician changing filter on the PDM mass sensor.**

### **Flow Measurement and Control**

Downstream of the mass sensor, the filtered airstream flows through an orifice used in conjunction with a differential pressure measurement to determine the volumetric flow rate. In-line relative humidity (RH) and temperature sensors are located ahead of a computer-controlled sample pump that generates the vacuum needed to sample the mine atmosphere. Other sensors measure the ambient temperature in the vicinity of the cyclone as well as the atmospheric pressure in the mine. The PDM uses these inputs, together with the sample airstream temperature measured close to the flow-measurement orifice, to determine the flow rate passing through the HD cyclone. A feedback loop in the PDM uses this information to dynamically control the speed of the pump so that the constant 2.2 L/min volumetric flow rate required for proper dust size separation is maintained at the cyclone, under the mine's ambient temperature and pressure conditions.

### **Battery Configuration**

The two identical battery packs inside the PDM provide power to the miner's cap lamp and the particle sampling and analysis system. The batteries can be recharged from a complete discharge in about 6 hr to provide maximum use of the monitor. The batteries make use of the latest lithium-ion technology used in portable computers to provide high-power density and superior charging and life cycle characteristics. The energy storage density enabled by lithium-ion battery technology allows for the packaging of a dust sampling and analysis system together with the batteries required for the cap lamp in a size and weight approximating those of the current battery pack. The PDM as tested weighed 3.0 kg (6.6 lb).

## Data Treatment

A microprocessor-based controller collects real-time inputs from sensors and the microbalance to provide a minute-by-minute record of the dust loadings and mine environment to which a miner is exposed. The PDM continuously displays personal dust exposure information to the miner in numeric and graphic formats and internally stores a full record of detailed data for about 20 full-shift sample runs. These data may be selected for downloading and analysis.

An illuminated data display on the top of the PDM continuously shows the previous 30 min dust concentration, cumulative mass concentration to that point in the shift, and an estimated EOS projected concentration exposure. Through the display, miners can gauge their current dust exposure, as well as the effectiveness of actions taken to reduce their dust exposure.

The exposure data described above are always displayed to miners, but are protected from tampering by being accessible only to an authorized person. In addition, the PDM allows miners and management to initiate short-term mass concentration measurements for specific monitoring objectives without affecting the shift-based statistics. This can be helpful to gauge the effectiveness of various dust or ventilation engineering control techniques. These intrashift measurements may be made as often as desired, and data obtained during these trials may be selected for downloading together with the tamper-resistant shift-based information.

## TEOM Mass Measurement Technique

At the heart of the TEOM mass sensor is a hollow tube, called the tapered element, which is clamped at its base and free to oscillate at its narrow end. The exchangeable filter cartridge mounted on its free end collects the respirable particles contained in the airstream that passes from the entrance of the mass sensor through the tapered element. Electronic components positioned around the tapered element cause the tube to oscillate at its natural (or resonant) frequency and at a constant amplitude. As additional mass collects on the sample filter, the natural oscillation frequency decreases as a direct result. This approach uses first principles of physics to determine the mass change of the collection substrate (filter) and is not subject to uncertainties related to particle size, color, shape, or composition.

The PDM determines the mass concentration of respirable dust in the mine environment by dividing the mass (as determined by the frequency change) collected on its filter over the air volume sampled during the same period. The system updates its mass concentration readings, shown in milligrams per cubic meter, every few seconds. The manufacturer uses NIST-traceable mass standards to calibrate the mass sensor constant  $K_0$ , which determines the relationship between mass change at the end of the tapered element and frequency change.

Filter mass is calculated every 5 sec according to

$$MT_0 = K_0 \times \left( \frac{1}{f_c^2} - \frac{1}{f_i^2} \right), \quad (1)$$

where  $MTO$  = mass;  
 $K0$  = the constant of the tapered element (TE);  
 $f_c$  = current frequency;  
 and  $f_i$  = initial frequency (i.e., at start of shift).

Mass rate and concentrations are derived from the mass, time, and flow rates of the instrument. Details of these calculations may be found in the PDM operations manual [Rupprecht and Patashnick Co. 2004].

### **Momentum Compensation: The Key to Miniaturization**

In the past, TEOM-based monitors were much too large and delicate to be used for personal exposure monitoring [Williams and Vinson 1986]. The potential for application of the TEOM technology to mining came through the miniaturization of the TEOM mass detector, which was made possible through the development of a patented concept involving momentum compensation. A momentum compensator built into the PDM mass sensor oscillates an additional mass at the same frequency, but in opposing phase to the tapered element. By applying this principle, energy loss from the tapered-element oscillator to its surroundings approaches zero with the appropriate design of the momentum compensator. The tapered element effectively behaves as if it were mounted on a massive base without the use of a large mass. The size and weight of the TEOM detector are dramatically reduced without compromising performance. In addition, the smaller sensor reduced the thermal heating requirements, enabling greatly reduced power consumption.

## **METHODS**

### **Laboratory Methods**

Performance of the precommercial series 3600 PDM was evaluated in the laboratory to validate instrument accuracy as received from the manufacturer and after use in mines. Using published criteria for comparing analytical techniques [Kennedy et al. 1995], NIOSH showed that for the prototype PDM, “there is a 95% confidence that the individual PDM measurements were within  $\pm 25\%$  of the reference measurements” and that the upper 95% confidence limit was met [Volkwein et al. 2004]. The precommercial 3600 PDM uses the identical mass measurement methods and algorithms as the prototype, and a detailed repeat of the entire accuracy evaluation was not warranted. However, to confirm this assumption, a limited version of the previous accuracy test was conducted with all of the new instruments.

### **Dust Exposure Chamber**

A laboratory Marple chamber provided a uniform test environment for comparing dust-measuring instruments while maintaining good control of test variables [Marple and Rubow 1983]. The chamber was operated to produce dust concentrations nominally ranging from 0.2 to 4 mg/m<sup>3</sup>. While this is the concentration range recommended in NIOSH’s *Guidelines for Air Sampling and Analytical Method Development and Evaluation* [Kennedy et al. 1995], it was

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

viewed as a guideline since it pertains to analytes that have very good reference standards. In our case, the reference was a gravimetric sampler. These samplers have been demonstrated [Kogut et al. 1997] to have significantly higher relative standard deviations (RSDs) in multiple sampler comparisons at mass concentrations of less than  $0.5 \text{ mg/m}^3$ . When reference mass loadings were less than  $0.5 \text{ mg/m}^3$ , the number of reference samples was increased to improve the accuracy of the reference mass measurement.

Chamber environment was regulated to between 20 and 25 °C and an RH between 40% and 60%. Instruments were mounted on a turntable in the Marple chamber that was rotated at a rate of one to two revolutions per minute. This eliminated the need for a randomized block design and ensured that each sampling device was exposed equally to all radial portions of the chamber.

Coal dust used in the chamber was from the Pittsburgh Seam having a median diameter of  $3.91 \text{ }\mu\text{m}$  with a geometric standard deviation (GSD) of 2.58. This dust was manufactured by passing the coal through an Alpine AFG Model 100 jet mill (Hosokawa Micron Powder Systems, Summit, NJ).

Chamber dust concentrations were monitored with a commercially available Model 1400a TEOM (TEC, Albany, NY). This was used to help select the correct time intervals to achieve desired mass loadings for the testing.

## Samplers

PDM mass measurement accuracy and precision were compared to the average of multiple gravimetric samples. A total of 25 PDMs were used as delivered by TEC. Samplers used for gravimetric analysis were BGI-4CP cyclones with integral filter holders (BGI, Inc., Waltham, MA) connected to MSA Escort Elf sampling pumps (MSA Co., Inc., Pittsburgh, PA). The BGI-4CP cyclone was an HD design, identical to that used in the PDM. The PDMs and the BGI-4CP cyclones were operated at 2.2 L/min. To further minimize test variables, the BGI-4CP samplers were modified to use an inlet and tube configuration identical to that in the PDMs.

### *PDM*

The PDM used Teflon-coated nominal 15-mm-diam filter media TX40H120WW (Pallflex Products Corp., Putnam, CT), manufactured into special plastic holders that mounted on the end of the hollow tapered element. This is the same filter medium used in the TEC Model 1400a ambient air monitor. The PDM sampler flow rate was checked and recalibrated if flow variance was greater than  $\pm 0.022 \text{ L/min}$ . Data on the flow rate and calibration of each instrument were recorded. Unfortunately, our records were incomplete for some of the units that were sent to the manufacturer for repairs. As a result, the analysis of flow rate stability was based upon 10 PDM units for which complete flow calibration histories were known.

PDM samplers were cleaned after each day of use. Cleaning consisted of removing the cyclone grit pot, removing the TE sensor module, and removing the filter on the TE. Canned compressed air was then blown from the cap lamp located inlet tube toward the cyclone, up the cyclone from

the grit pot, and from the TE connection back toward the cyclone. The TE module and cyclone grit pot were then cleaned with the compressed air. A new filter was installed on the TE, and the module and cyclone grit pot were reattached to the PDM.

### *Gravimetric Reference*

The filters used in the BGI-4CP cyclone were 37-mm-diam, 5- $\mu$ m pore size, polyvinyl chloride (PVC) membranes. Flow-controlled MSA Elf Escort pumps were calibrated on-site at the beginning of each group test using a Gilibrator (Sensidyne, Inc., Clearwater, FL) primary standard flow meter to  $2.2 \pm 0.022$  L/min for the BGI-4CP samplers. An equivalent pressure restriction for the respective samplers was used during pump calibration.

### *Impactors*

Size distributions of the dust in the chamber were measured using a Marple personal cascade impactor (Model 290, TEC, Franklin, MA) operated at a flow rate of  $2.0 \pm 0.020$  L/min using Elf Escort pumps. The device was operated according to the manufacturer's instructions, including correction factors to account for inlet efficiency and wall loss [Rubow et al. 1987].

The impactor has eight collection stages with cut points from 0.7 to 21.3  $\mu$ m and a final filter (PVC 37-mm-diam, 5- $\mu$ m pore size). At each collection stage, dust particles impact on a 34-mm-diam Mylar® substrate at six impaction zones. Before using the substrates, the impaction zones were coated with grease to hold the collected particles on the substrates. This was done by covering the 34-mm-diam Mylar substrate with a metal template that has six slots that expose the impaction zones. These slots were then sprayed with a 1- to 10- $\mu$ m-thick layer of impaction grease (Dow Corning 316 Silicone Release Spray, Dow Corning Corp., Midland, MI). After spraying, the substrates were kept at constant temperature and humidity for 3 days to allow the volatile components of the silicone spray to evaporate and to outgas. The substrates and the PVC final filters were then preweighed and loaded into the eight stage impactors. Impactors were used in triplicate to measure the size distribution of the coal dust. Three substrates and three final filters were used as blank controls.

The size distribution mass median aerodynamic diameter (MMAD) and GSD were determined from a straight line regression of impactor stage data plotted as the inverse cumulative distribution function of the normal distribution or probit of cumulative mass percentages versus the logarithm of stage cut point [Hinds 1982]. The use of least squares regression to find the best-fitting straight line for this type of plot is recommended only if the regression is truly linear because it overemphasizes the tails of the distribution. Cumulative lognormal plots often show curvature toward the tails, resulting in regression error of the distribution parameters. To account for this, data were used only if the  $R^2$  values for the regression were greater than 0.95.

### **Analytical Gravimetric Precision**


Gravimetric analysis was performed on a Cahn C-31 microbalance for the impactor samples and a Mettler-Toledo UMT2 microbalance for the BGI-4CP and CMDPSU samples. Weighing was



done in the NIOSH PRL laboratory at  $73 \pm 0.7$  °F and  $53 \pm 2$  % RH. All samples were pre- and postweighed using control filters. Average blank control filter weights were used to correct the filter mass results for each test employing impactors, BGI-4CP, and the CMDPSU. However, cyclic fluctuations in these conditions are not totally accounted for by the control filters for two reasons. First, the control filters cannot be weighed at the same time as the sample filters. Secondly, the pre- and postweighings are not performed at the same time in relation to the cyclic variation of the room conditions. Therefore, several estimates for the weighing precision will be provided.

## Experimental Design

Because of the limited weight and volume capacity of the Marple chamber, the 25 PDMs were divided into two groups of 12 and 13. Three replicate test runs were conducted with each group. Each individual test run used 15 BGI-4CP samplers. The inlets of all samplers were uniformly arrayed around a central point in the Marple chamber (Figure 4).

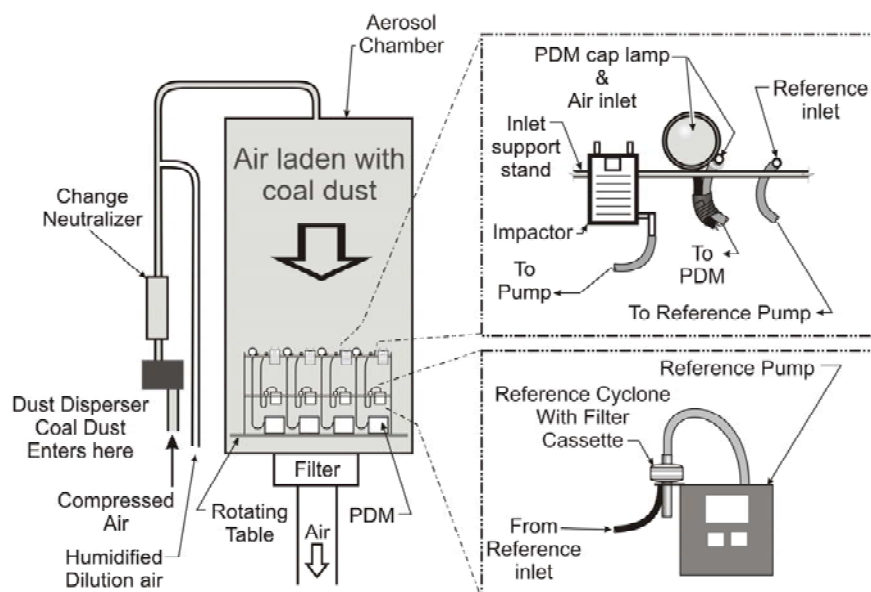

**Figure 4.—Laboratory test chamber and arrangement of instruments.**

The 15 gravimetric samplers were divided into four test-time interval groups. The first time interval used six samplers to account for the increased variability of the reference measurement when mass loadings were less than  $0.5 \text{ mg/m}^3$ ; the second, third, and fourth time intervals used three samplers.

The mass collected by the samplers in each time group was used to determine the average reference gravimetric dust mass during a specific test-time interval. In addition, there were three

blank control filters for each test. Control filters were handled in an identical fashion to the test filters, except that the cassette end caps were not removed. Final test filter weights were corrected using the average control filter change in mass.

We selected test-time intervals to achieve filter mass target loadings over the range of about 0.2–4 mg. For a typical test run, the internal computer for each PDM was programmed to automatically start and all gravimetric samplers were manually started at the same time. Because of the large number of gravimetric samplers started manually, they were started sequentially by group and stopped in the same sequence to minimize any time differences between samplers caused by starting and stopping. As mass loaded onto the samplers with time, groups of gravimetric sampling pumps were turned off at predetermined mass loadings as indicated by the Model 1400a TEOM using an HD cyclone at a flow rate of 2.2 L/min. The mass loading therefore determined the test-time interval. This procedure resulted in four test-time intervals with averaged mass loadings from corresponding groups of BGI-4CP samplers. For each test-time interval, the PDM mass recorded in each data file was read to determine the mass measured by the individual PDM for that test-time interval.

The three test runs were essentially replicates except that the mass loadings varied as follows:

- *Run 1.*—8-hr duration, test-time interval Nos. 1–4. The chamber was brought to a concentration of about 2 mg/m<sup>3</sup>. Gravimetric filters were turned off at equivalent mass target loadings of 0.4, 0.9, 1.4, and 2 mg. Impactor size distribution samples were taken with three impactors to confirm that the size distribution of this study was comparable to previous sizes associated with this coal type.
- *Run 2.*—8-hr duration, test-time interval Nos. 5–8. The chamber was brought to a concentration of about 4 mg/m<sup>3</sup>. Gravimetric filters were turned off at equivalent mass target loadings of 1, 2, 3, and 4 mg.
- *Run 3.*—8-hr duration, test-time interval Nos. 9–12. The chamber was brought to a concentration of about 2 mg/m<sup>3</sup>. Triplicate sets of filters were turned off at equivalent mass target loadings of 0.2, 0.7, 1.7, and 2.0 mg.

## **PDM Battery Test**

Previous work had demonstrated that the lithium-ion batteries used in the PDM could enable a 12-hr sample to be taken, but did not address what happens to PDM performance as batteries weaken prior to failure. A test was conducted with six PDMs to monitor mass rate of accumulation and flow rate as the instruments' batteries ran out of power. This laboratory test established a dust concentration of 2 mg/m<sup>3</sup> in the Marple chamber that was continuously monitored using a Model 1400a TEOM and PDMs that were run to battery failure.

## **PDM Mass Constant Verification**

During this evaluation, we verified the mass constant of the PDM. To determine mass, each individual tapered element (TE) used in a PDM has an empirically derived mass constant.

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

### *Definition of Constant*

The constant  $K0$  ( $K$  zero) is determined by recording the TE's frequency change due to a known mass applied to the TE's filter and inputting data into the following equation:

$$K0 = \frac{m}{\left(\left(1/f_f^2\right) - \left(1/f_i^2\right)\right)}, \quad (2)$$

where  $K0$  = the constant of the TE;  
 $m$  = the mass in grams added to the TE filter;  
 $f_i$  = the baseline frequency in hertz of the TE before the mass is added;  
 and  $f_f$  = the frequency in hertz of the TE after the mass is added.

The  $K0$  for each TE was determined by averaging five  $K0$  measurements. The  $K0$  was calculated each time the mass on the TE was changed. The resulting average was then compared with the  $K0$  that had been programmed by TEC into each PDM.

### *Procedure to Determine Mass Constant*

All of the PDMs were cleaned and had new filters inserted on their TEs. Their inlets were connected to a HEPA filter to eliminate the possibility of dust contamination. Throughout the tests, all of the PDMs were connected to their battery chargers/computer connection, which enabled real-time graphing of the TE frequency. The PDMs were run for a minimum of 1 hr for warmup before any  $K0$  measurements were made.

The known masses added to the TE filter were small, preweighed aluminum tabs with adhesive on one side of the tab to couple the tab to the filter surface. The tabs were preweighed just before the tests in the controlled atmosphere of the PRL weighing lab.

After warmup, the PDMs were programmed with the WinPDM 5.12 expert software program to activate the mass frequency template and to display and log data every second. The software program graphed the frequency curve in real time. By observing this curve, we could determine when the frequency had stabilized. The stabilized baseline frequency ( $f_i$ ) was recorded. The tapered-element module was removed from the PDM, and a preweighed aluminum tab was attached near the center of the TE filter. The tapered-element module was then reinserted into the PDM and the frequency curve observed. Once the frequency had stabilized, the new frequency ( $f_f$ ) was recorded along with the mass of the aluminum tab. This process was repeated five times. Each additional piece of aluminum mass was uniformly distributed across and adhered to the filter. Mass at each frequency was the summation of the individually added pieces. The  $K0$  for each mass was then calculated according to formula 2 and the average  $K0$  of the five readings calculated. This averaged  $K0$  was then compared with the  $K0$  that had been programmed into the PDM.

## Analysis

The accuracy and precision were calculated from the data pairs of individual PDM mass measurements to the average gravimetric reference standard. Accuracy, bias, and precision were calculated by the method of Kennedy et al. [1995]. For these tests, the mass ratio for each data pair was calculated by dividing the individual PDM mass by the average value for the triplicate gravimetric reference mass measurements of the corresponding time interval. The individual mass ratios were then averaged over each group of data. The RSDs were calculated for both PDM and gravimetric reference standards. To reduce the impact of error in the gravimetric reference measurement, the experimental pooled estimate of the RSD of the gravimetric samplers was subtracted from the RSD of the ratios such that the corrected RSD was

$$RSD_x = \sqrt{RSD_{\frac{x}{t}}^2 - RSD_{T_i}^2}, \quad (3)$$

where  $RSD_{\frac{x}{t}}$  = relative standard deviation of mass ratio

and the experimental pooled RSD of the gravimetric samplers was

$$RSD_{T_i} = \frac{\sqrt{\frac{\sum RSD_{gravimetric}^2}{n}}}{2} \quad (4)$$

Bias was then calculated based on the mean concentration minus one. Accuracy was calculated based on the method provided by Kennedy et al. [1995]. Confidence limits were calculated based on the method used by Bartley [2001] using the noncentral Student's  $t$ -distribution.

The precision of the PDM was analyzed for each test by examining the RSD of the PDM and reference samplers over mass loadings ranging from 0.2 to 4.3 mg. To determine the overall precision of the PDM from the premine laboratory data, an RSD was computed using a one-way analysis of variance (ANOVA). The intratest RSD was estimated by the square root of the mean square error (RMSE). The dependent variable for this analysis was the dust concentration measured in milligrams per cubic meter, and the independent (or grouping) variable was the laboratory test. There were six tests with 12–13 PDMs per test. For each test, dust concentration measurements were collected at four time intervals. For each PDM, the dust measurements were averaged across the time intervals within each individual test. In order to be consistent with the methodology used to calculate the PDM field precision, the concentration measurements were log-transformed (log base  $e$ ) before the analysis was conducted.

## Detailed In-mine Test Methods

In this portion of the study, PDMs were used by miners to estimate the long-term mechanical, functional, and ergonomic features of the samplers. The in-mine precision of the PDM and reference samplers was determined.

### Criteria for Mine Selection

This testing required a high level of cooperation from the host mine to permit training, allocate working space, and commit labor to maintain the PDMs in the absence of NIOSH personnel. The level of cooperation required precluded choosing mines at random for this portion of the testing. Mines were, however, selected to include a variety of coal types, machine types, geographic locations, seam heights, and workforce size. Representative geographic distribution of mines was achieved by selecting one mine from each of the 10 MSHA bituminous coal mining districts. Table 1 shows the characteristics of each mine. Within this sample, we then selected by type of machine and by on-section locations to obtain dust samples that were representative of where miners work.

**Table 1.—Detailed mine characteristics and location of Lippmann sample**

MSHA district	Mine height, in	Mining method	Distinguishing features	Location of sample
2.....	65	CM	Exhaust vent tube, integral miner bolter.....	On miner left rear side.
3.....	70	CM	Exhaust vent tube, integral miner bolter.....	On miner near left bolter.
4.....	65	LW	PDM powered remote .....	Shield 30.
5.....	48	CM	Scrubber, bridge face haulage .....	Immediate miner return.
6.....	56	CM	Small mine.....	Bolter.
7.....	50	CM	Pillar section – retreat ventilation to gob.....	Behind miner toward gob side.
8.....	46	CM	Super section single split vent, low coal .....	Immediate miner return.
9.....	120+	LW	High seam .....	Shield 20.
10.....	46	CM	Low coal, super section .....	Immediate miner return.
11.....	72	CM	Diesel face haulage.....	Twin boom bolter.
CM Continuous mining.		LW Longwall.		

### Detailed Mine Procedures

At each detailed mine test site, NIOSH spent 3 days on-site to demonstrate and teach mine personnel how to use and maintain the PDM. Sampling of an entire face crew was conducted over the miners' entire work shift, which includes travel to and from the working section. In addition, the precision of triplicate samplers was determined. The PDMs were then left at 6 of the 10 mines for use by the mine without NIOSH present. At the end of the 10th detailed mine study in late spring of 2005, four mining companies conducted extended testing of the PDM at their mines to further evaluate the stand-alone performance of the instrument.

At each mine, NIOSH presented a 45-min training session at the start of the shift. The training contained a short video to ensure that information was presented in a uniform manner. A pocket-

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

sized memory jogger card was given to each miner wearing a PDM to remind them about the points discussed on the video. The mine section where miners were to wear the PDM was selected by management and hourly employee representatives. In addition to the section crew, management and labor representatives and safety personnel attended the training. NIOSH provided additional training to the mine employees who would maintain the PDMs at the mine.

Data collected at each mine included the full-shift dust exposure of each miner, the corresponding MSHA occupation code, and a notation of any problems in collecting the data. Mine personnel programmed the PDMs to automatically start sampling at the beginning of the shift and to sample for the entire shift length. Between 7 and 14 PDMs were used depending on the size of the section crew. Each day, miners picked up their assigned PDM as they would have normally picked up their cap lamps and returned the PDMs to the charger at the end of the shift. A mine employee would then download the data, clean the inlet tube and cyclone, change the filter, and program the samplers for the next shift of sampling. Data from the samplers were considered valid when the PDM ran for the entire shift with no mechanical or electronic faults, or human errors. This mechanically correct sample could later be considered void in the event that the data file showed a flow fault or other sampling abnormality. The number of mechanically correct samples divided by the total number of samples attempted to be taken during a shift determined the overall valid or sampling success rate for this testing. Subsequent analysis of the data file may determine that a sample should be voided for cause, but this would not affect the overall valid sampling rate. Flow rates for these PDM samplers were considered acceptable at  $\pm 5\%$  of 2.2 L/min. In the event that the PDM flow sensor was greater than  $\pm 0.2$  L/min of the calibrated flow for a period of 60 sec, the PDM would place an error message on the display in the file for later evaluation of the severity of the fault.

For the first 3 days of sampling, NIOSH personnel collected area samples, were present on-site to help with the PDM sampling, and accompanied the miners underground to answer questions. At the first six mines, NIOSH left all of the PDMs for the section crew at the mine site under the supervision of the mine. The same section of miners continued to use the PDMs for the next week. If a miner was absent, the miner's replacement would wear the PDM. Similarly, if the entire crew changed from day to evening shift, the PDMs stayed with that crew to maintain consistency. If extra instruments were available, other miners working outby would occasionally wear a PDM. The following week, NIOSH returned to the mine and accompanied the section crew to work. NIOSH observed and talked to miners about their experience with the PDM. We then collected the instruments and data records. This resulted in 8–11 shifts of data from each PDM from every member of the mining section. The variable number of days resulted from some mines continuing testing through the weekend or scheduled shift changes.

## Area Sampling

Area sampling was conducted for 3 days at each mine to determine the precision of the PDM, DO cyclone, and impactor size distribution measurements. A stationary Lippmann-type sampling apparatus [Blachman and Lippmann 1974; Volkwein and Thimons 2001] was used to collect triplicate measurements from the PDM, Marple personal impactors, and CMDPSUs at flow rates of 2.0 L/min and 1.7 L/min. The Lippmann device minimized spatial variability

associated with mine sampling. Weighing and calibration procedures for this testing were identical to the laboratory testing. The 3 days of sampling conducted in 10 mines resulted in a total of 30 triplicate measurements from which the precision of instruments was calculated. A preliminary regression analysis between the PDM and CMDPSU was done.

## **Maintenance and Use Log**

Over the course of the research, all usage of the project's 25 PDMs was recorded. A chronological record was kept for each PDM unit summarizing the number of hours it actively ran from its delivery date to the end of the project. This included all types of laboratory and field operation, regardless of the nature of the usage, test, or monitoring being performed. Therefore, for the purpose of summarizing overall PDM use, only total hours logged was considered, and the environment or nature of differing instrument deployments was not a distinguishing factor.

Each PDM also had its individual repair history recorded, which included some details of problems experienced and repairs performed to resolve the problems. For these repair records, distinctions were made between types of manufacturer repair. Repairs were categorized as either remedial or critical. Remedial repairs reflected current or pending hardware or software modifications to instrument design, minor in nature, that were unlikely to be ongoing issues once fully instituted. Examples of remedial repairs include updating firmware to correct performance problems, correcting manufacturing defects, and replacing failed faceplate keypads or display screens. Critical repairs were defined as repairs necessary for full functional operation of the instrument to collect valid data. Critical repair frequency was regarded as somewhat more reflective of ultimate instrument reliability after design refinements.

Further maintenance log entries were also made to record success or failure of each PDM run. If a PDM completed a run with valid data, the run was evaluated as a success. If a run was not completed, or a data file was electronically corrupted, the run was evaluated as a failure. While the nature of run failures was recorded, types of failures were not subcategorized. Researchers intervened and corrected unsuccessful PDM performance as soon as problems were recognized. In many instances, minor adjustments were adequate to resolve instrument problems. Less frequently, manufacturer service was required and recorded.

## **Field Precision Analysis**

In order to determine the precision of the PDM, the DO cyclone at 2.0 L/min, and the DO cyclone at 1.7 L/min, the RSD was computed using a one-way ANOVA. To determine the within-day variability average among the triplicate samplers, a technique using the standard deviation calculated from the ANOVA was used to compute the RSD. Because the distributions of the dust concentrations for each sampler were positively skewed, the data values were log-transformed (log base  $e$ ) before the analysis. The dependent variable for this analysis was the dust concentration measured in milligrams per cubic meter, and the independent (or grouping) variable was the date of the in-mine sampling test. There were 30 unique dates with triplicate measurements collected on each date for each instrument type.

## RESULTS

### Laboratory Accuracy Verification

Evaluation of the data from the prototype PDM to determine whether it met the NIOSH accuracy criterion has been reported by Volkwein et al. [2004]. The limited lab testing reported here is intended to verify that the precommercial 3600 PDM maintained similar performance to the prototype PDM before field use of the instrument.

#### Premine Testing

Premine accuracy verification test results in Table 2 present the average mass of dust from the BGI-4CP samplers for each test-time interval, the corresponding individual PDM mass measurements by serial number, and the RSD of both samplers. The overall average RSD for the gravimetric reference sampling for these laboratory samples is 0.041 for the first group of tests and 0.039 for the second group. The RSD for the PDM units for each test-time interval is indicated; the average RSD for these measurements was 0.057 for the first group of tests and 0.043 for the second group. The RSD of the combined data calculated for the PDM was equal to 0.051 (95% CL = 0.048, 0.057). This value will be subsequently used in the discussion of the calculation of field precision.



**Table 2.—Premine laboratory data of reference mass measurements and PDM mass measurements**

Time interval	Gravimetric avg. mass, mg	RSD	PDM mass by serial number													RSD
			110	112	113	115	119	126	127	128	130	131	132	133	135	
			mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	
1	0.426	0.048	0.377	0.406	0.384	( <sup>1</sup> )	0.409	0.388	0.359	0.431	0.413	0.393	0.414	0.357	0.381	0.058
2	0.968	0.047	0.901	0.956	0.903	( <sup>1</sup> )	0.958	0.903	0.939	0.992	0.952	0.897	0.967	0.843	0.881	0.046
3	1.506	0.033	1.384	1.481	1.397	( <sup>1</sup> )	1.483	1.397	1.462	1.515	1.453	1.363	1.481	1.289	1.354	0.048
4	2.184	0.023	1.931	2.054	1.942	( <sup>1</sup> )	2.053	1.933	2.036	2.108	2.020	1.887	2.064	1.792	1.884	0.048
5	1.132	0.033	1.050	1.066	0.994	0.955	1.052	1.047	1.013	1.124	1.033	1.009	( <sup>1</sup> )	0.935	1.061	0.050
6	2.160	0.049	2.104	2.163	1.991	1.929	2.098	2.115	2.032	2.254	2.097	2.000	( <sup>1</sup> )	1.839	2.115	0.054
7	3.244	0.054	3.075	3.161	2.910	2.833	3.068	3.110	2.976	3.298	3.076	2.923	( <sup>1</sup> )	2.658	3.087	0.055
8	4.308	0.036	3.980	4.090	3.757	3.675	3.970	4.027	3.843	4.271	3.989	3.795	( <sup>1</sup> )	3.425	3.975	0.056
9	0.193	0.082	0.196	0.202	0.201	0.202	0.212	0.196	0.204	0.205	0.222	0.197	0.203	0.165	0.214	0.066
10	0.747	0.021	0.732	0.732	0.733	0.727	0.774	0.732	0.741	0.757	0.800	0.701	0.759	0.596	0.797	0.069
11	1.796	0.033	1.688	1.700	1.702	1.689	1.792	1.697	1.720	1.776	1.837	1.637	1.788	1.396	1.833	0.066
12	2.144	0.033	1.967	1.984	1.975	1.959	2.076	1.968	1.993	2.072	2.139	1.909	2.074	1.633	2.124	0.064
Average gravimetric RSD		0.041	Average PDM RSD													0.057

Time interval	Gravimetric avg. mass, mg	RSD	PDM mass by serial number													RSD	
			102	105	108	109	111	114	116	120	122	123	124	125	115		132
			mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg		mg
1	0.424	0.069	0.410	0.377	0.376	0.432	0.451	0.395	0.427	0.391	0.430	0.426	0.372	0.411	0.400		0.061
2	1.003	0.025	0.914	0.854	0.860	0.967	0.989	0.887	0.971	0.889	0.960	0.960	0.840	0.925	0.901		0.054
3	1.572	0.034	1.454	1.354	1.376	1.508	1.571	1.406	1.544	1.415	1.521	1.515	1.331	1.481	1.433		0.052
4	2.115	0.034	1.990	1.865	1.917	2.055	2.149	1.927	2.125	1.949	2.076	2.082	1.836	2.037	1.973		0.049
5	1.111	0.044	1.055	1.008	0.993	1.009	1.089	1.011	1.095	1.059	1.028	1.108	1.048	1.076		1.066	0.035
6	2.169	0.002	2.024	1.928	1.918	1.930	2.097	1.957	2.108	2.035	1.974	2.131	2.016	2.070		2.055	0.036
7	3.224	0.042	2.999	2.890	2.874	2.864	3.130	2.914	3.124	3.028	2.961	3.159	2.978	3.067		3.058	0.034
8	4.213	0.030	3.846	3.709	3.689	3.683	4.002	3.744	4.012	3.891	3.814	4.046	3.809	3.927		3.916	0.032
9	0.185	0.076	0.203	0.202	0.192	0.199	0.204	0.191	0.205	0.194	0.198	0.203	0.181	0.218			0.045
10	0.724	0.025	0.730	0.721	0.692	0.717	0.736	0.703	0.758	0.710	0.724	0.750	0.676	0.768			0.037
11	1.814	0.040	1.742	1.722	1.646	1.702	1.777	1.673	1.798	1.685	1.722	1.772	1.613	1.839			0.038
12	2.035	0.051	2.005	1.985	1.893	1.969	2.041	1.936	2.075	1.952	1.987	2.043	1.867	2.117			0.037
Average gravimetric RSD		0.039	Average PDM RSD													0.043	

<sup>1</sup>Test run in group 2.

The size distribution of the coal dust in the chamber had an MMAD of 3.91  $\mu\text{m}$  and a GSD of 2.58. This was comparable to the intermediate-sized Pittsburgh coal dust used in determining accuracy of the prototype instrument [Volkwein et al. 2004].

## Postmine Testing

Postmine testing accuracy verification data in Table 3 show the average mass of dust from the triplicate BGI-4CP samplers for each test-time interval, the corresponding individual PDM mass measurements, and the RSD of both samplers. The overall average RSD for the gravimetric reference sampling for this work was 0.039 for the first group of tests and 0.049 for the second group. The RSD for the PDM units for each test-time interval is indicated; the average RSD for these measurements was 0.056 for the first group of tests and 0.051 for the second group. The size distribution of the coal dust for postmine testing had an MMAD of 4.01  $\mu\text{m}$  and a GSD of 2.53.

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

Table 3.—Postmine laboratory data of reference mass measurements and PDM mass measurements

Time interval	Gravimetric avg. mass, mg	RSD	PDM mass by serial number													RSD
			102	108	112	113	114	115	119	120	123	124	125	127	128	
			mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	
1	0.425	0.026	( <sup>1</sup> )	0.373	0.445	0.397	0.359	0.386	( <sup>1</sup> )	0.410	0.404	0.405	0.429	0.418	0.388	0.058
2	0.960	0.030	( <sup>1</sup> )	0.817	0.953	0.861	0.788	0.832	( <sup>1</sup> )	0.895	0.880	0.885	0.932	0.892	0.850	0.053
3	1.475	0.065	( <sup>1</sup> )	1.281	1.463	1.344	1.220	1.278	( <sup>1</sup> )	1.368	1.369	1.365	1.438	1.373	1.328	0.048
4	1.950	0.029	( <sup>1</sup> )	1.717	1.955	1.794	1.629	1.720	( <sup>1</sup> )	1.827	1.833	1.833	1.923	1.822	1.777	0.046
5	1.012	0.049	0.885	0.875	0.995	0.890	0.824	0.865	0.931	0.982	0.946	0.931	1.010	0.947	0.924	0.064
6	1.931	0.038	1.759	1.741	1.972	1.764	1.638	1.740	1.859	1.947	1.870	1.843	1.995	1.891	1.833	0.061
7	2.899	0.033	2.639	2.608	2.958	2.656	2.460	2.627	2.789	2.919	2.809	2.763	2.981	2.827	2.751	0.060
8	3.906	0.038	3.576	3.512	3.997	3.601	3.329	3.566	3.757	3.938	3.801	3.741	4.011	3.821	3.730	0.058
9	0.209	0.048	0.185	0.173	0.202	0.189	0.162	0.179	0.193	0.197	0.191	0.190	0.184	0.193	0.189	0.061
10	0.709	0.047	0.669	0.621	0.692	0.652	0.585	0.647	0.673	0.701	0.707	0.689	0.661	0.675	0.658	0.054
11	1.738	0.042	1.601	1.506	1.672	1.568	1.420	1.560	1.620	1.667	1.714	1.647	1.580	1.628	1.591	0.052
12	2.114	0.028	1.874	1.772	1.963	1.848	1.664	1.836	1.907	1.964	2.000	1.940	1.856	1.913	1.865	0.051
Average gravimetric RSD		0.039	Average PDM RSD													0.056

Time inter- val	Gravi- metric avg. mass, mg	RSD	PDM mass by serial number														RSD
			105	109	110	111	116	122	126	130	131	132	133	135	102	119	
			mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	mg	
1	0.395	0.044	0.361	0.355	0.353	0.323	0.378	0.385	0.371	0.367	0.329	0.342	0.336	0.353	0.363	0.378	0.053
2	0.962	0.062	0.831	0.800	0.786	0.728	0.843	0.869	0.823	0.817	0.758	0.771	0.752	0.786	0.830	0.864	0.053
3	1.425	0.007	1.283	1.228	1.205	1.128	1.313	1.340	1.276	1.272	1.173	1.188	1.169	1.226	1.275	1.328	0.052
4	2.096	0.040	1.854	1.758	1.734	1.617	1.890	1.936	1.838	1.829	1.690	1.719	1.671	1.766	1.837	1.913	0.054
5	1.031	0.029	0.912	0.850	0.844	0.795	0.940	0.931	0.900	0.895	0.889	0.852	0.854	0.888			0.047
6	2.061	0.036	1.856	1.692	1.696	1.590	1.900	1.868	1.804	1.803	1.785	1.716	1.699	1.771			0.051
7	2.909	0.023	2.788	2.519	2.521	2.363	2.825	2.783	2.696	2.696	2.652	2.568	2.523	2.625			0.052
8	3.901	0.093	3.712	3.360	3.371	3.173	3.786	3.721	3.595	3.602	3.573	3.428	3.372	3.502			0.052
9	0.183	0.078	0.175	0.174	0.170	0.163	0.169	0.180	0.189	0.185	0.187	0.180	0.169	0.188			0.049
10	0.722	0.125	0.637	0.583	0.580	0.578	0.613	0.654	0.667	0.637	0.633	0.608	0.595	0.638			0.049
11	1.772	0.020	1.554	1.405	1.385	1.389	1.482	1.582	1.598	1.528	1.524	1.458	1.425	1.539			0.051
12	2.146	0.027	1.853	1.666	1.650	1.652	1.762	1.890	1.907	1.822	1.813	1.740	1.693	1.839			0.052
Average gravimetric RSD		0.049	Average PDM RSD														0.051

<sup>1</sup>Test run in group 2.

## Accuracy

The premine test results support the thesis that design changes made between the prototype PDM–1 and the precommercial 3600 PDM did not affect the accuracy of the instrument. Results from the pre- and postmine calculation of bias, precision, accuracy, and 95% upper confidence limits (UCLs) are shown in Table 4. The bias results show that the PDM reads consistently less than the gravimetric reference mass measurement. Despite the bias, high precision enables the point estimate of accuracy to meet the  $\pm 25\%$  criterion. However, there were occasions for both the pre- and posttesting when the results failed to meet the 95% UCL that the PDMs are within  $\pm 25\%$ . Failure of an instrument to meet the 95% UCL but to not exceed a 5% CL (failure to meet criterion) results in the decision that the accuracy determination for those samplers is inconclusive. Of particular note for the postmine testing was that bias values greater than  $-0.13$  were associated with all instruments that did not meet the 95% UCL for reasons to be discussed.

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

**Table 4.—PDM pre- and postmine lab accuracy calculations**

PDM No.	Premine lab tests				Postmine lab tests			
	Bias	Precision	Accuracy	Upper 95% confidence limit	Bias	Precision	Accuracy	Upper 95% confidence limit
102.....	-0.04	0.05	12	18	-0.10	0.02	12	14
105.....	-0.08	0.07	18	26	-0.10	0.03	13	16
108.....	-0.09	0.05	16	21	-0.13	0.02	15	17
109.....	-0.05	0.06	14	20	-0.16	0.05	22	27
110.....	-0.06	0.03	11	15	-0.16	0.05	23	27
111.....	0.00	0.04	8	11	-0.20	0.04	25	28
112.....	-0.03	0.03	7	10	-0.01	0.03	5	8
113.....	-0.07	0.05	14	19	-0.09	0.01	10	11
114.....	-0.08	0.04	13	18	-0.18	0.02	20	22
115.....	-0.08	0.06	17	22	-0.11	0.02	14	15
116.....	0.00	0.04	7	11	-0.10	0.05	16	21
119.....	-0.02	0.05	10	15	-0.07	0.02	9	11
120.....	-0.06	0.04	12	16	-0.04	0.03	8	11
122.....	-0.04	0.05	11	16	-0.07	0.02	11	13
123.....	-0.01	0.03	7	10	-0.05	0.02	8	10
124.....	-0.10	0.04	16	20	-0.06	0.01	7	7
125.....	-0.01	0.07	14	21	-0.03	0.06	12	18
126.....	-0.06	0.03	10	14	-0.09	0.04	15	20
127.....	-0.06	0.05	14	20	-0.05	0.02	8	10
128.....	0.01	0.02	4	6	-0.08	0.02	11	12
130.....	-0.01	0.07	13	20	-0.11	0.04	17	21
131.....	-0.09	0.04	14	18	-0.13	0.07	22	28
132.....	-0.02	0.03	7	10	-0.15	0.05	22	26
133.....	-0.18	0.04	22	25	-0.17	0.04	22	25
135.....	-0.04	0.07	16	24	-0.12	0.05	19	24

Even though some of the units' postmine sampling accuracy results were inconclusive, the mean accuracy values of pre- and postmine testing are statistically equal. Results from an independent samples t-test show mean accuracy (premine) = 12.271 (95% CL = 10.517, 14.025) and (postmine) = 14.674 (95% CL = 12.213, 17.081) (t-value (df = 48) = -1.63, p-value = 0.11). The null hypothesis that the mean premine accuracy is equal to the mean postmine accuracy was not rejected.

One PDM failed to meet the 95% UCL of accuracy during the premine testing and was returned to the factory for examination and recalibration. We were unable to verify that the factory's recheck restored accuracy; consequently, this unit was not used for underground precision determination. However, the postmine verification testing showed that the sampler in question was within the accuracy criterion.

### Calibration Constant $K_0$

We investigated why some instruments did not meet the posttest 95% UCL. Table 5 presents the results of the laboratory measurement of the constant factor ( $K_0$ ) that the instrument uses to calculate mass from the change in frequency of the tapered element. The RSD of replicate measurements of  $K_0$  conducted with two of the instruments was 0.0038 and 0.0027.

**Table 5.—Comparison of PDM measured  $K_0$  and programmed  $K_0$** 

Unit No.	Premine lab tests		Postmine lab tests		Measured $K_0$	Programmed $K_0$	$K_0$ difference, %
	Accuracy, %	Upper 95% confidence limit	Accuracy, %	Upper 95% confidence limit			
119.....	10	15	9	10	15368	15427	-0.4
127.....	14	20	8	9	15138	15552	-2.7
112.....	7	10	5	8	15827	16028	-1.3
112.....	Rep	Rep	Rep	Rep	15719	16028	-2.0
112.....	Rep	Rep	Rep	Rep	15724	16028	-1.9
110.....	11	15	23	27	15166	13846	8.7
131.....	14	18	22	28	15138	14827	2.1
133.....	22	25	23	26	15107	14361	4.9
132.....	7	10	22	26	14534	13846	4.7
132.....	Rep	Rep	Rep	Rep	14537	13846	4.8
132.....	Rep	Rep	Rep	Rep	14466	13846	4.3

Rep Replicate  $K_0$  measurement.

We compared the  $K_0$  factor for units with higher and lower posttest accuracy. For three PDMs with lower or better UCL accuracy during the postmine testing, the programmed  $K_0$  was within 2.7% of the measured  $K_0$ . However, for four of the PDMs that did not meet the postmine test UCL accuracy (i.e., higher), the difference in the measured  $K_0$  from programmed  $K_0$  showed a reduction by as much as 8.7%. Further investigation of the data file logs also revealed that for some of the PDM units, the programmed  $K_0$  factor was changed by the factory between the pre- and posttesting when the units were returned for repair. Not all units needed this recalibration. However, any instrument that had a repair in the TE module (i.e., temperature sensing) may have required the  $K_0$  to be recalibrated. Because the constant is directly proportional to mass, this recalibration may be one reason why the postmine testing did not meet the 95% UCL for accuracy. Bias introduced by the calibration constant causes some of the inaccuracy observed.

### Limit of Detection and Quantification

Determination of the traditional limit of quantification (LOQ) [Marple and Rubow 1983] requires determining the standard deviation of weighing ( $S_W$ ) in nine consecutive weighings of a blank filter. Both balances were determined, coincidentally, to have  $S_W = 1.4 \mu\text{g}$  and a resultant  $\text{LOQ} = 14 \mu\text{g}$  in a single weighing. However, quality control procedures involving control room filters used only in the balance room document that the total standard deviation ( $S_T$ ) due to  $S_W$  and the cyclic fluctuations in weigh room conditions during the course of this study was  $S_T = 4.1 \mu\text{g}$ . Applying traditional formulas for propagation of error in the filter dust weight gains, we obtain  $S_{\text{filter}} = 2S_T = 8.2 \mu\text{g}$ . The factor 2 results from the fact that there are four weighings required to determine the mass gain of the sample: the pre- and postweighing of both the sample and the control filter average. Similarly, for the calculations derived from the impactor, given that there are 9 stages involving 36 weighings, we obtain  $S_{\text{impactor}} = 6S_T = 24.6 \mu\text{g}$ .

## Battery Depletion Effects

There was no detectable effect on instrument accuracy, as batteries were intentionally run to failure. The frequency measurement by the TE was unaffected by small drops in battery voltage. Comparing the mass accumulation rate of an individual PDM with a corresponding TEOM 1400a, there was no change in the slope as batteries failed. The most significant effect measured as battery power fails was the decreased flow associated with the pump. Figure 5 shows that the flow diminished from full nominal flow rate of  $2.2 \text{ L/min} \pm 5\%$  to  $0 \text{ L/min}$  in less than 2 min. The resulting change in the cyclone classification as a result of the low flow condition represented about 0.3% of an 8-hr sample time. The data also showed that one instrument failed 518 min into the test. The battery charger cable to this instrument was faulty and was replaced prior to additional testing.

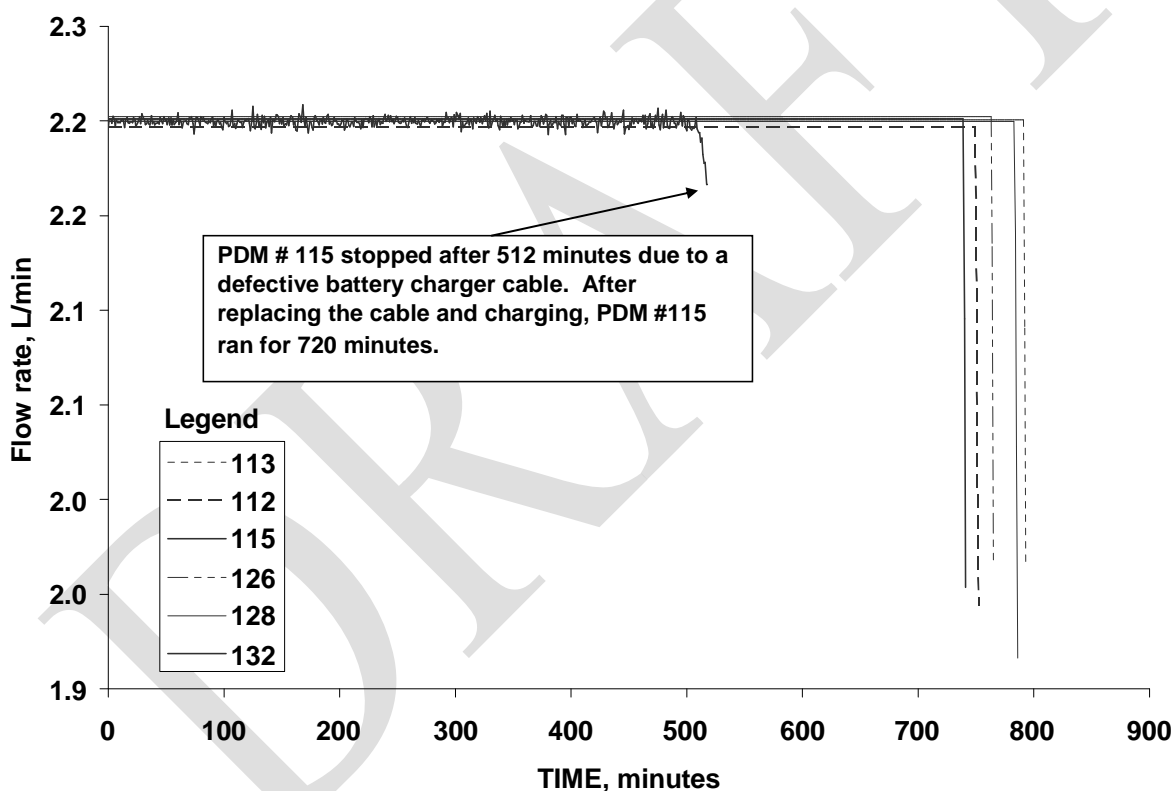


Figure 5.—Battery testing to failure using flow rate as an indicator.

## Detailed In-mine Testing

### Performance Over Project Duration

Testing was conducted from November 2004 to August 2005. Results in Table 6 show the total number of samples taken with PDMs in each of the MSHA districts sampled, the number of valid samples recorded, the percentage of valid samples, and a breakdown of whether NIOSH personnel were present or absent on the property. Valid concentration data for each occupation at each of the detailed mine sites are in Appendix A. The data were collected during typical mining operations, and data collection was not associated with any negative consequences for the mines. The data represent an overall performance rate of the software, electrical, mechanical, and physical subsystems of the PDM. At the first mine site, a significant error in the internal instrument software resulted in multiple errors and an instrument availability for valid data collection of 51%. All instruments were returned to the manufacturer for reprogramming. Subsequent testing proceeded with average instrument availability of 93% with a range between 86% and 97%.

**Table 6.—Total samples taken during detailed mine sampling and number of valid samples when NIOSH was present or absent from the mine property**

MSHA district	NIOSH present			NIOSH absent			Total		
	No. samples	No. valid	% valid	No. samples	No. valid	% valid	No. samples	No. valid	% valid
<b>DETAILED MINE TESTING</b>									
9.....	31	17	55	64	31	48	95	48	51
3.....	30	29	97	37	33	89	67	62	92
4.....	27	22	81	45	40	89	72	62	86
11.....	40	39	98	64	59	92	104	98	94
2.....	36	34	94	60	53	88	96	87	91
10.....	35	35	100	68	63	93	103	96	93
6.....	30	28	93				30	28	93
5.....	33	32	97				33	32	97
8.....	38	37	97				38	37	97
7.....	23	22	96				23	22	96
<b>EXTENDED MINE TESTING<sup>1</sup></b>									
2(1).....				9	4	44	9	4	44
9(1).....				22	20	91	22	20	91
2(2).....				26	23	88	26	23	88
9(2)a.....				7	7	100	7	7	100
9(2)b.....				9	3	33	9	3	33

<sup>1</sup>For the extended mine testing within MSHA districts 2 and 9, each district had two companies ("1" and "2"). Within district 9, company 2 sampled at two mines ("a" and "b").

After testing at the sixth mine site, the percentage of valid samples with NIOSH present or absent showed little difference. NIOSH, in consultation with the PDM Partnership, concluded that the remaining detailed mine testing did not require the second week of testing, and the remaining detailed mine site testing was conducted for only the 1 week with NIOSH present. Testing concluded in May 2005, followed by a period of extended mine testing.

## Extended Testing

A period of extended mine sampling was conducted from June to August 2005. Results of instrument availability in Table 6 are similar, but more variable than the previous detailed mine results. This was caused primarily by one PDM at mine 2(1) and another PDM at mine 9(2)b that failed for the entire trial periods, where mine staff were untrained to recognize such problems. Consequently, mine staff continued to run instruments that normally would not have been used. The problem with each instrument was, however, obvious when downloaded data files were examined.

Feedback from the miners using the PDM during the extended mine testing was consistent with the feedback received during the detailed mine testing, although not all mines provided written feedback to NIOSH. Comments from miners are in the “Discussion” section of this report. A new issue raised during this testing was that the side entry of the power cord into the cap lamp was not compatible with the flip clip used on the personal air purifying respirators in use at one mine. The flip clip relies on the in-line tension of the cap lamp power cord to maintain the light position when the face shield is raised. The side entry of PDM cap light creates an off-balance situation.

## Maintenance Results

The 25 precommercial PDM instruments logged 10,926 hr of testing, of which 8,023 hr were conducted underground. The average logged use per instrument was 437 hr, with a maximum of 644 hr and a minimum of 246 hr. Hours of use varied based on the type of sampling for which each particular unit was used. The earliest repair episodes before the firmware upgrade were not counted in final PDM repair summaries, as they were regarded only as factory adjustments to the released product.

Table 7 presents the summary of PDM use and repair. Each PDM unit is listed with actual total hours and categorized repairs. Total repair rates and critical repair rates per 1,000 hr of projected instrument use are presented in the table. Data for individual PDMs are ordered first by best critical repair rate and next by best total repair rate. The 25 PDMs are divided into quintiles of 5 PDMs each, with best repair rates at the top of the table. Summary averages are recorded by quintile groups and also for the full set of all 25 PDMs.

Repair frequency varied among the precommercial PDMs. Those in the top two quintiles needed little service, while those in the bottom two quintiles required more repairs by the manufacturer. The bottom quintiles required both remedial and critical repairs. However, the top quintiles only required repairs of a remedial nature. The PDM instruments in the top quintile averaged 506 hr of use without needing a critical repair. Their ultimate reliability could not be calculated because no critical repairs were required for them over the full timespan of the project.

Table 8 presents the summary of PDM run success rates for all PDM sampling. Each PDM unit is listed with its count of total runs and successful runs. An invalid run can be caused by human error, such as poor filter placement, in addition to a mechanical failure. Data are ordered by best

success rate, with highest percentage rates at the top of the table. Data are again organized by quintile groups, with summary data for all 25 PDMs also recorded. The overall average success rate was 90.18% based on 1,202 total runs. The run success rates for the top two quintiles ranged from 92.42% to 100.00%. Data from Tables 7–8 are independent assessments of instrument reliability. Consequently, repair rates do not correspond to run success rates in part because of researcher intervention to prevent accumulation of unsuccessful samples. In addition, the causes of failed runs were often minor and readily correctable without manufacturer repair.

**Table 7.—Summary of PDM use and repair by quintile**

PDM No.	Total repairs	Remedial repairs	Critical repairs	Total hours run	Total repairs/1,000 hr	Critical repairs/1,000 hr
111.....	1	1	0	612.25	1.63	0.00
114.....	1	1	0	512.00	1.95	0.00
135.....	1	1	0	505.00	1.98	0.00
126.....	1	1	0	482.25	2.07	0.00
130.....	1	1	0	418.50	2.39	0.00
Means.....	1.00	1.00	0.00	506.00	2.01	0.00
125.....	1	1	0	392.50	2.55	0.00
124.....	1	1	0	390.75	2.56	0.00
115.....	1	1	0	315.25	3.17	0.00
116.....	2	2	0	581.25	3.44	0.00
127.....	1	1	0	246.00	4.07	0.00
Means.....	1.20	1.20	0.00	385.15	3.16	0.00
112.....	2	2	0	445.75	4.49	0.00
120.....	2	2	0	416.25	4.80	0.00
131.....	2	2	0	384.50	5.20	0.00
128.....	3	3	0	328.25	9.14	0.00
133.....	2	1	1	643.75	3.11	1.55
Means.....	2.20	2.00	0.20	443.70	5.35	0.31
102.....	2	1	1	581.00	3.44	1.72
122.....	3	2	1	515.25	5.82	1.94
123.....	2	1	1	408.25	4.90	2.45
105.....	2	1	1	406.00	4.93	2.46
113.....	3	2	1	399.25	7.51	2.50
Means.....	2.40	1.40	1.00	461.95	5.32	2.22
119.....	2	1	1	383.50	5.22	2.61
132.....	3	2	1	373.00	8.04	2.68
110.....	4	3	1	361.00	11.08	2.77
109.....	3	1	2	503.50	5.96	3.97
108.....	3	1	2	321.25	9.34	6.23
Means.....	3.00	1.60	1.40	388.45	7.93	3.65
Summary means.....	1.96	1.44	0.52	437.05	4.75	1.24



**Table 8.—Overall success rate**

PDM No.	Total count	No. valid	% valid
131.....	42	42	100.00
135.....	56	55	98.21
108.....	36	35	97.22
127.....	33	32	96.97
105.....	43	41	95.35
Mean.....			97.55
126.....	49	46	93.88
116.....	61	57	93.44
125.....	45	42	93.33
114.....	55	51	92.73
111.....	66	61	92.42
Mean.....			93.16
132.....	39	36	92.31
102.....	64	59	92.19
112.....	51	47	92.16
128.....	33	30	90.91
119.....	39	35	89.74
Mean.....			91.46
123.....	47	42	89.36
122.....	56	50	89.29
115.....	42	37	88.10
133.....	70	61	87.14
109.....	54	47	87.04
Mean.....			88.18
130.....	46	40	86.96
110.....	37	31	83.78
120.....	46	38	82.61
124.....	45	36	80.00
113.....	47	33	70.21
Mean.....			80.71
Total.....	1,202	1,084	
Mean.....			90.18

## Underground Precision

Statistical results from the ANOVA in Table 9 show RSDs of the instruments in the Lippmann chamber used in the detailed mine sampling. All data used in this analysis are in Appendix B. The PDM had an RSD of 0.078 with a 95% CL of 0.066–0.095. Kissell and Sacks [2002] state that for normally distributed data, a 25% accuracy criterion is met with an RSD of 0.125 or less. The CMDPSU at a flow rate of 2.0 L/min had an RSD of 0.052, which can be compared to previous work by Kogut et al. [1997] where an RSD of 0.046 was determined for the same sampler at weight gains of greater than 0.5 mg/m<sup>3</sup>. The higher RSD of 0.082 for the CMDPSU at a flow rate of 1.7 L/min is caused by a few influential samples that looked anomalous, but had no physical reason to be excluded from the data set.

**Table 9.—Field precision results**

Instrument	No. of samples	RSD	95% CL
PDM.....	88	0.078	.066–.095
CMDPSU: 2.0 L/min flow rate.....	89	0.052	.044–.063
CMDPSU: 1.7 L/min flow rate.....	90	0.083	.070–.101

## DISCUSSION

### Training and Comments

Training sessions on how to use the PDM at each mine were 30–45 min long. This training was important not only to ensure that miners knew how to use the PDM, but also to offer the opportunity for NIOSH to answer miners' concerns and objections. Miners were encouraged to provide us with their opinions and feedback on their experiences with the PDM.

A key feature of the PDM is that it must be suitable for use by miners. In addition, miners for the first time have a timely way of accurately knowing the dust levels in their work environment. During the course of the study, NIOSH had an opportunity to informally listen to miners' opinions about the PDMs while they were wearing and working with the units. This part of the discussion relates anecdotes recorded by the researchers during the testing. The initial reaction to the PDM during the introduction and training session of the detailed mine visits was one of skepticism and doubt about the size, weight, cap light, and overall benefit of the instrument. By the end of the detailed mine testing, most miners felt that they would prefer their dust monitoring be done with the PDM mainly because it did not interfere with their work in the way the current sampler does.


The reaction of miners varied from total disinterest, where they treated the PDM just like their cap lamp, to active involvement where they were correlating what they were doing with what the instrument was telling them. One miner operator said that he glanced at the display after every shuttle car of coal. The data from the PDM offered some surprises to the miners. Some roof bolters expressed surprise that they were “getting dust when they could not see it.” A rock duster said he was surprised that his levels were so low when conditions appeared particularly dusty. Most of the miners who paid attention to the PDM thought it was a useful tool. One foreman used the results of the shuttle car operators to change their routes to minimize exposures.

There were several comments that the curved design of the PDM offsets the slight increase in the weight of the unit over the weight of the lead-acid cap lamp batteries currently used by all of the mines in these trials. One complaint, particularly by the mechanics, was that the PDM was bulkier than the lead-acid batteries and that there was less room for tools on the belt. Miners commented that the quality and brightness of the cap lamp was good, but many did not like the nonfocusable lens system, particularly if the light was not focused correctly. Miners generally preferred the old-style, full-size backup bulb in the cap light over the white LED lamp in the PDM. One mine suggested that the LED bulb should be green to help see in smoke. Unlike feedback during the prototype testing, there were few complaints about the noise of the pump.

Occupations in outby areas were more likely to comment about the noise than face workers. Noise was more noticeable during dinner break, but not objectionable. The pump outlet that produces most of the noise is highly directional and easily muffled with a coat without affecting the flow. Frequent complaints were made that the cap lamp cord was too long. The longer-length cord was selected for these trials to ensure that the length would accommodate the largest miners. In fact, when shorter cords were installed for the extended mine testing, complaints resulted that the cords were too short. Cord length of production units should be easily exchangeable. Another complaint about the cords was that they were stiff and chafed the necks of miners in warmer mines.

### Screen Presentation of Data

The data display screens, shown in Figure 6, show the miner his or her exposure data in different formats. Miners responded differently to this information. Some found value in the graphic format; others preferred one of the numeric formats. The nomenclature used to describe each of the numeric formats caused confusion. Based on observations in this testing, the cumulative concentration (CUM0), which is mathematically the mass divided by volume sampled to this point in time, becomes a good predictor of the EOS concentration about midway through the shift, provided that conditions do not change. On the other hand, the projected concentration (PROJ), which is mathematically the mass divided by the volume to be sampled for the entire shift, is not a direct estimate of a miner's EOS concentration. Perhaps a better name for this value is "limit concentration." Regardless of the name, the worth of the "PROJ" value is that it will not fluctuate with changes in the concentration; rather, it steadily progresses to the true EOS concentration. If CUM0 exceeds the permissible exposure limit (PEL), steps can be taken to reduce the exposure to stay within the PEL before the EOS. Once the limit (PROJ) is exceeded, it becomes impossible to meet the PEL. Despite the apparent confusion in nomenclature, miners watching the screens quickly learned to identify the meaning of the various formats in relation to their activities.

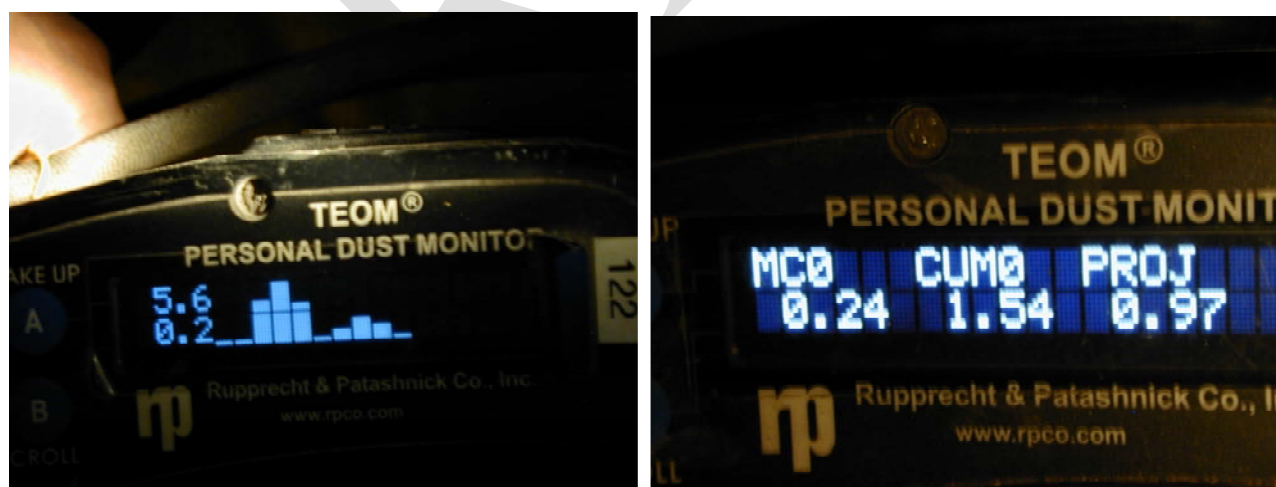

**Figure 6.—Basic PDM screen display formats and information presented. Left: graphic format; right: numeric format.**

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

## Performance Issues

During mine testing, small engineering and operational issues occurred that may have affected the availability of the instrument for use or were reported as a nuisance by the miners. Table 10 reports those issues and steps taken to resolve them. As with any new system, especially those used by miners in the challenging underground environment, operational issues such as these will only be discovered through use of the device. The introduction of the currently used CMDPSU into the mining industry underwent several years of issue discovery and problem-solving until the technology matured. The testings of the prototype and the current precommercial PDM have probably not identified all of the possible issues with this new technology, but hopefully have helped shorten the time in which full maturity will be reached.

**Table 10.—PDM performance issues and comments**

Performance issue	Comments
Control of TE temperature.....	Resolder connection of temperature sensor; heater was OK.
Display malfunction.....	Poor quality control from supplier; hired new supplier – replaced all keypads or fuses.
Button malfunction .....	Part of display assembly replaced.
PDM failed to communicate to computer .....	Software/firmware bug fixed by TEC after first mine trial.
Battery failure .....	Replaced battery.
Premature cap lamp bulb failure .....	Reengineer filament thickness. Resubmit for MSHA approval.
Flat line in data file .....	Intermittent problem; unresolved – possible incorrect filter placement.
Low power.....	Associated with charging problems; bad battery cell or insufficient charging.
Charger problem, contacts give false indication of charge status.	Clean contacts, design contacts to be self-cleaning. Improve charger-sensing firmware.
High filter load at start of test.....	Incorrect filter placement.
Broken cyclone inlet .....	Add better strain relief at inlet.
Cut tube at cyclone inlet.....	Add better strain relief at inlet.
Bad focus on cap lamp.....	Reshim bulb; instruct technician on focus procedures.
TE not detected.....	Design tighter TE connection.
Failed leak checks.....	Connection between cyclone and PDM leaks; resealed with silicone grease, needs redesign.
Incompatible with new remote controls .....	TEC to redesign power output cable of PDM to remote to be compatible with new devices.
Cable to cap lamp too long or too short .....	TEC to offer alternative lengths or be capable to field retrofit.

## Data Files

### Download

When WinPDM software is used to download data from the PDM to the computer, several options are available to the user. The first option is to print a “dust data card” (Figure 7), which looks similar to the currently used dust data card, but contains the final EOS exposure of the instrument and any error codes recorded by the instrument. In this case, the actual exposure was  $0.73 \text{ mg/m}^3$ . The instrument currently reports how each sample was terminated in the error code field. In this example, a normal program end of sample message appears in the error code field. Since normal termination of a sample is not an error, this message is inappropriate for that field. The next option during downloading is to visually examine graphs of various parameters such as concentration, mass, flow, pressure, or tilt versus time. This option was not frequently used in this testing, but was useful to provide a quick summary of the day’s events. Finally, the data can be saved by the computer in a comma-separated version (.CSV) text file for archiving or more detailed examination using common spreadsheet software.

Dust Data Card: (Serial Number 0123)

1. Wearer ID  
1036

2. Mine ID Number  
01 00759

3. Contractor Code  
000

4. Mine Name  
[redacted] #1

5. Company Name  
[redacted]

6. Date Sampled  
01 25 05

7A. Sampling Start Time  
06

7B. Sampling Time (min)  
480

8. Time This Shift

9. Type of Sample (select one)  
(1) designated occ (ug) ☐ 0  
(2) nondesignated occ (ug)  
(3) designated area (ug)  
(4) designated work position  
(5) part 90 miner

10. MMU DA/SA  
017 0

11. Occ Code  
036

12. Part 90 Miner Sampled  
SSN [redacted]

13. Certified Person: NOTICE - Knowingly making any false statement, representation, or certification on this document is a violation of the federal criminal code which may be punished by a fine or by imprisonment or both.  
SSN [redacted]

Signature  
X

14. Results  
Actual Exposure: 0.733831 mg/m<sup>3</sup>

15. Errors  
14:00:01 01/25/2005, Program end of sample

Notes:  
[redacted]

**Figure 7.—Example of data printout. (MMU = mining machine unit. DA = designated area. SA = surface area.)**

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

## Interpretation

Data graphs can be constructed from the text files. Figure 8 shows the results of a plot of the data created from a saved file associated with the dust data card from Figure 7. These data illustrate the effect of a short-term dust spike at 9:00 on the cumulative and projected dust concentrations. The cumulative concentration decreases after the spike, but the projected concentration continues to increase. At the end of the shift, the cumulative and projected concentrations are equal.

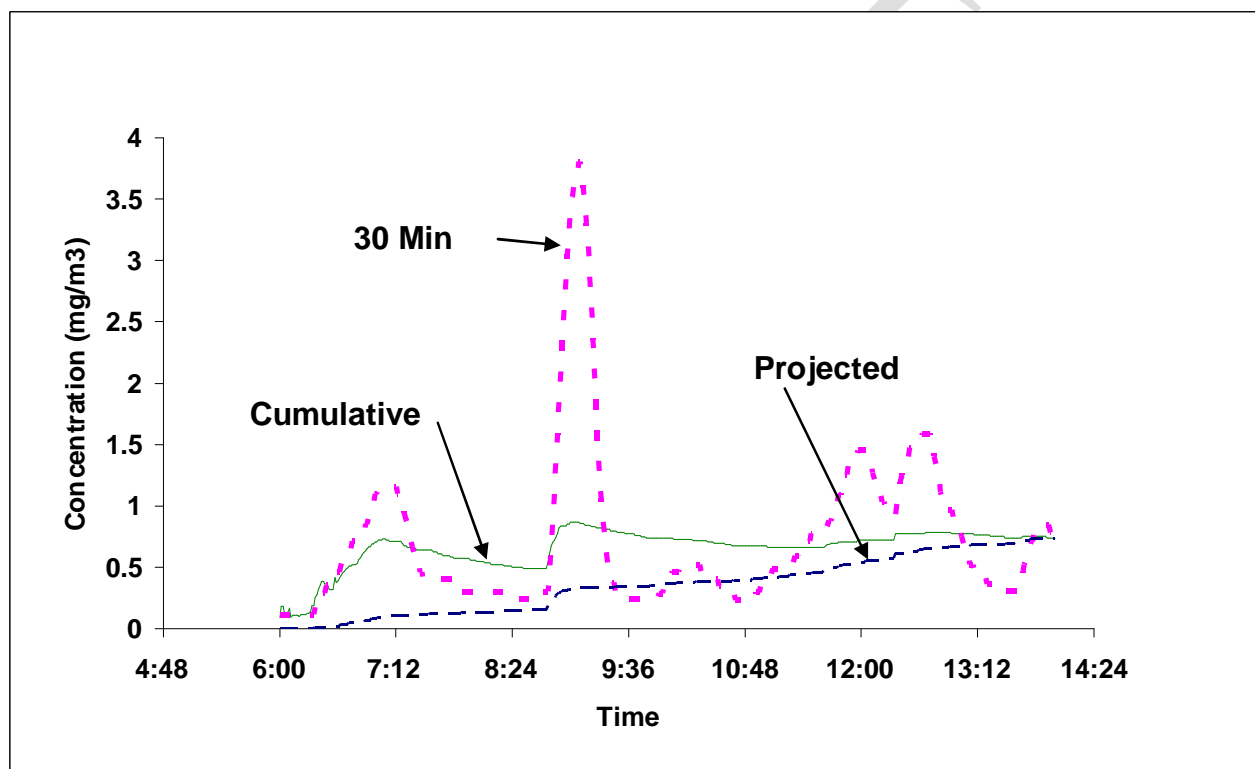


Figure 8.—Detail of results from sample shown in Figure 7.

## Error Codes

### Meaning and Interpretation

The PDM automatically senses and has the capability to report many useful instrument and environmental parameters. These parameters may be selected by the factory or authorized user and can be stored in memory with the frequency or change interval desired. TEC provides a basic template of settings and a diagnostic template for troubleshooting the device. This template can be configured to report error flags at various settings.

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*


## Distinguishing Valid Data

How these error code parameters are set to distinguish valid from invalid samples is an important question. The criteria for selecting the validity of a sample will ultimately lie with the end use of the instrument. A difference between the prototype and precommercial PDM was the way in which errors were determined. The original thinking to distinguish one type of valid from invalid samples was to use the tilt sensor to determine if the instrument was inverted and consequently dislodged oversize particles from the cyclone grit pot onto the mass sensor (a rare occurrence based on the data in Appendix C). Prototype results indicated that this was not a reliable method since it gave frequent false indications. In addition to being nonrespirable, oversize particles invalidate a sample under the current system because it results in an excessive, instantaneous mass increase to the filter. As an alternative to using the tilt function, a new algorithm was written for the precommercial PDM in which the rate of mass increase of the filter would result in a mass offset (MO) error being reported. Thus, the result of the tilt event—oversize changing the mass on the filter—rather than the event itself becomes the reason for invalidating a sample.

In this testing, the MO sensitivity settings were initially set to report an error when the mass loading increased by 50  $\mu\text{g}$  over a 2-min time interval. At this setting, MO errors were frequently reported when in fact valid data were being recorded, such as when entering a return airway. This setting was changed after the second mine trial to only report errors when a level of 100  $\mu\text{g}$  over a 1-min time interval was sensed. This change greatly reduced the frequency of MO errors. However, valid data were still being reported as an error, and a higher mass loading setting is probably warranted.

In addition, when the sample inlet tube is pinched closed, the resulting sudden decrease in pressure in the TE environment is sensed and is reported as a rapid change in mass, resulting in a MO error. This is evident in Figure 9 where the differential pressure and mass are plotted. Note that when the pinch is relieved, the mass returns to the original level so that the EOS concentration measurement is unaffected by the event. We also note that these pinch events may momentarily reduce the flow rate of the instrument. With this information, the manufacturer should be able to refine the MO algorithm to ignore events when a pressure spike occurs. If the resulting pinch continues for 2 min, a flow error will occur and the sample may be invalidated for that reason. Similarly, the algorithm could be refined such that if an MO event occurs and a tilt event also occurs, then a tilt error could be recorded as the reason to invalidate a sample.



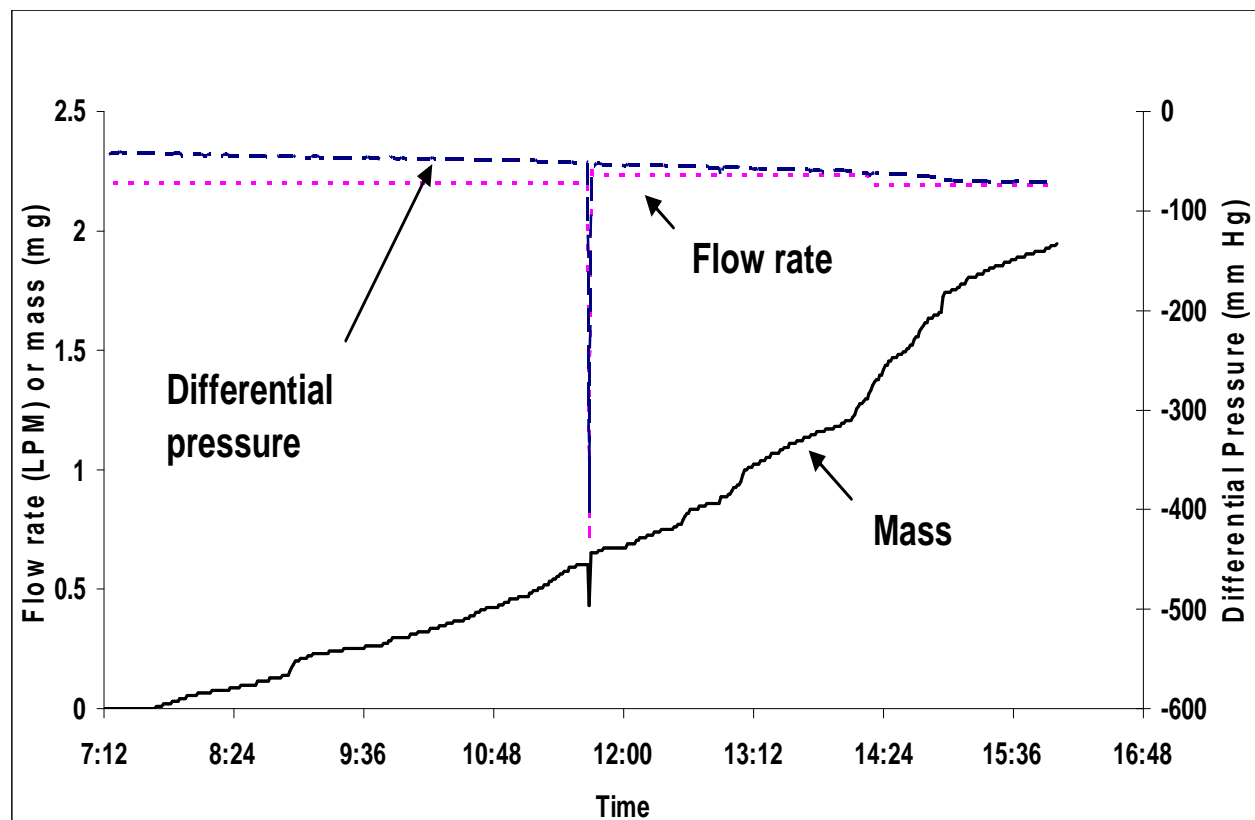

**Figure 9.—Mass offset "error" resulting from pinched tube and subsequent recovery of correct mass measurements.**

MSHA currently uses a system of void codes to detect events such as those just mentioned. Analysis of MSHA data (Appendix C) for the 10-year period from 1994 to 2004 shows conventional filter sampling success (nonvoid) rates for inspector and operator samples of 92.3% and 83.1% on total samples of 381,335 and 487,713, respectively. Based on the type of void rates and the expanded capabilities of the PDM, we estimate that about half of the MSHA voided samples could have been valid samples using PDM technology.

### **Instrument Bias Sources**

At the outset of this work, certain technical tradeoffs were made in order to make the measurement of coal mine dust exposure both functional and accurate. One acknowledged tradeoff is the loss of respirable dust in the tube from the cap light to the cyclone. This source of loss was minimized through the use of conductive tubing, which minimized electrostatic losses, and by the use of an optimized transport velocity. Peters and Volkwein [2003] calculated and measured this loss to be about 2% of the total respirable fraction. Another source of particle loss may occur in the heater between the cyclone and PDM filter. This has not been quantified

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

directly, but is a part of the overall measurement of bias. The measured bias of the PDM is negative and thus consistent with the physical loss of a small amount of particulate mass in the transition zone between the cyclone and filter. This loss will be variable depending on the respirable size distribution of the dust. Results from both the laboratory and the detailed testing in this work indicate that various particulate losses within the PDM are trivial. The technical tradeoffs made to create a more functional instrument have had a minimal impact on instrument comparison to established sampling techniques.

The cause of the increase in the bias of the postmine accuracy verification testing may have arisen from three separate or combined sources. The first is that the *K0* calibration value differences have some association with high bias values of some but not all of the instruments. Secondly, the manufacturer discovered that the gasket between the cyclone and PDM could expand (creep) into the dome transition area and disrupt the flow in that area, creating particulate loss. Finally, it was observed in one of the units that did not meet the 95% UCL that a sealant had contaminated the conical cyclone outlet, which would contribute to the creation of turbulence and particulate loss. Regardless of the cause, periodic calibration of the instrument is advisable.

### **Maintenance**

Ongoing refinements to instrument design make remedial type of service, required in this study, less likely for future manufactured instruments. It is reasonable to expect that further refinements to design and manufacturing quality will ultimately cause all PDM units to perform in a manner consistent with the higher quintiles of these preproduction units once all issues related to minor design remediation and manufacturing practice are addressed.

### **Calibration**

#### **Flow**

PDM flow rates did not require frequent calibration. The initial flow calibration of each PDM occurred in late fall of 2004, when all units were returned to the manufacturer for firmware upgrades. Hours logged before this calibration are not included in this analysis. Recalibrations and hours logged are counted from the firmware upgrade service date onward. Two error standards for flow variance from the 2.2 L/min nominal flow rate were maintained for this testing. A  $\pm 1\%$  standard was used for laboratory and precision testing, and a  $\pm 5\%$  standard was used for the other detailed mine testing because this is the current allowable variance for CMDPSU sampling. Table 11 shows the calibration, flow error, and hours-logged histories for the 10 PDM units with complete flow calibration histories. Each PDM is taken as having an initial manufacturer flow calibration, with a few units also experiencing subsequent researcher recalibration of flow. Only one PDM required recalibration to maintain  $\pm 5\%$  flow rate. Three PDMs were recalibrated to meet the more stringent  $\pm 1\%$  calibration requirement for the research portion of the testing. A total of 3,354 hr were logged for the 10 PDM units.

**Table 11.—Flow calibration history**

PDM No.	1%–5% flow recalibration	>5% flow recalibration	Total hr run
111.....	0	0	459.25
114.....	0	0	455.50
135.....	0	0	392.25
126.....	0	0	321.75
130.....	0	0	299.75
125.....	0	0	339.25
124.....	0	1	264.50
115.....	1	0	204.25
116.....	0	0	419.75
127.....	2	0	197.75
Totals .....	3	1	3,354.00
Hours per calibration to maintain $\pm 1\%$ flow.....			239.57
Hours per calibration to maintain $\pm 5\%$ flow.....			838.50

Currently, MSHA inspectors and mine operators calibrate flows for personal sampling pumps after each 200 hr of use. Although Table 11 cannot indicate a definitive timespan for scheduling periodic instrument flow calibrations, it does provide a reasonable range. Approximately 240 hr per calibration occurred for the 10 PDMs examined to meet a  $\pm 1\%$  criterion, and approximately 840 hr per calibration occurred to meet a  $\pm 5\%$  criterion. We would project from this information that calibration of flow should occur between 240–840 hr. PDM flow stability is at least as reliable as current pumps and should not require more frequent calibration than current operator sampling procedures.

## Mass

Routine laboratory measurement of mass requires that the balances used to measure mass be periodically calibrated to ensure the validity of the measurement. The PDM will likewise need to be periodically audited to ensure the validity of the measurement. The change in bias with use observed in this testing suggests that the frequency of this calibration be done on a periodic basis. This initially should be done on the same time basis as the flow rates are checked. As more experience with the PDM is gained, this time period for checking mass calibration could be revised.

## Precision

It has been suggested that the field precision of the PDM should be adjusted to account for instruments that may be delivered from the manufacturer that did not meet the initial NIOSH accuracy criterion. The logic for this adjustment is that most users would be unable to detect such flaws and that this would actually be a contributing factor in the precision calculation. The adjusted RSD would be calculated from

$$RSD_{new} = \left( RSD_{field} + \frac{n_{fail}}{100n_{total}} \left( \frac{RSD_{field}}{RSD_{lab}} \right) \right) \quad (5)$$

Only one PDM failed to meet the initial 95% UCL accuracy criterion. The high precision of the lab measurements result in a small change of field precision from 0.0780 to 0.0786. Furthermore, these first instruments were in the precommercial stage of production, and one might expect the manufacturer's quality control to improve with experience, further reducing this impact on the field precision.

## CONCLUSION

An accurate direct-reading dust monitor for use in coal mines has been demonstrated in laboratory and underground coal mine environments. Through a protocol developed by a partnership of labor, government, and industry, this work verified that the laboratory accuracy met the criterion with 95% confidence that the individual PDM measurements were within  $\pm 25\%$  of the reference measurements. Accuracy after an extended period of mine use did not differ from the initial accuracy measurements. However, some individual units did exceed the 95% UCL after testing, and a shift in the bias of the instrument was a suspected cause. This leads to the recommendation that a calibration check of the instrument be part of the operating procedures. Mine data demonstrated that the precision of the PDM operating in coal mines had an RSD of 0.078.

Mine testing of the PDM when worn by miners during normal work demonstrated durable performance with about a 90% availability rate, which is similar to existing dust sampling devices. Many miners commented that they would prefer to use the PDM over the current sampler for dust measurements because of the integration of the sampler into the cap lamp and immediate access to the data. They further appreciated the immediate feedback of the screen-displayed exposure information. Some miners quickly learned to use the information to take action to minimize their exposures.

The final demonstration of equivalency to the MRE standard will be the subject of a subsequent publication.

Future work includes how miners might make use of the data from the PDM to actually lower exposures. A study will be conducted to document how miners make use of the new dust

exposure information they receive from their PDMs. Structured interviews will be conducted with approximately 50 miners representing each major category of underground mining job. Effective strategies for using PDM information will be documented, published, and shared throughout the coal industry. Although data were collected to measure the equivalency of the PDM to the MRE as required by U.S. law, the analysis of these data was more complex than originally anticipated because the increasing variance with concentration required use of a more sophisticated statistical model than originally planned. A second publication containing a detailed analysis comparing the PDM sampler used in this work to MRE and ISO standards is in progress.

## ACKNOWLEDGMENTS

The authors thank and acknowledge the support and technical advice provided by members of the PDM Partnership, namely, Dennis O'Dell of the United Mine Workers of America, Joe Lamonica of the Bituminous Coal Operators' Association, and Bruce Watzman of the National Mining Association. We also thank MSHA for its active support and participation in the collaborative research effort by purchasing units for testing and collecting vital test data at some 180 mechanized mining units around the country. We thank the individual mine managements for their hospitality and gratefully acknowledge the miners from the underground trials who worked hard to enable valid field data to be collected. We appreciate the generous engineering support provided by Erich Rupprecht, Business Development Manager, and Dan Dunham, PDM Project Manager, from Thermo Electron Corp. Finally, we thank Erica E. Hall, Calvin D. Garbowsky, Shawn E. Vanderslice, and Jeanne A. Zimmer of the NIOSH Pittsburgh Research Laboratory for their conscientious support in managing the logistics of the equipment for both the laboratory and mine measurements.

## REFERENCES

- Bartley DL [2001]. Definition and assessment of sampling and analytical accuracy. *Ann Occup Hyg* 45(5):357–364.
- Bartley DL, Chen CC, Song R, Fischbach TJ [1994]. Respirable aerosol sampler performance testing. *Am Ind Hyg Assoc J* 55(11):1036–1046.
- Blachman MW, Lippmann M [1974]. Performance characteristics of the multicyclone aerosol sampler. *Am Ind Hyg Assoc J* 35(6):311–326.
- CFR. Code of federal regulations. Washington, DC: U.S. Government Printing Office, Office of the Federal Register.
- Hinds WC [1982]. *Aerosol technology: properties, behavior, and measurement of airborne particles*. New York: John Wiley & Sons, Inc.
- ISO [1995]. *Air quality: particle size fraction definitions for health-related sampling*. Geneva, Switzerland: International Organization for Standardization. ISO 7708:1995.
- Kennedy ER, Fischbach TJ, Song R, Eller PM, Shulman SA [1995]. *Guidelines for air sampling and analytical method development and evaluation*. Cincinnati, OH: U.S. Department of Health and Human Services, Public Health Service, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, DHHS (NIOSH) Publication No. 95–117.
- Kissell FN, Sacks HK [2002]. Inaccuracy of area sampling for measuring the dust exposure of mining machine operators in coal mines. *Min Eng* 54(2):33–39.
- Kogut J, Tomb TF, Parobeck PS, Gero AJ, Suppers KL [1997]. Measurement precision with the coal mine dust personal sampler. *Appl Occup Environ Hyg* 12(12):999–1006.
- Marple VA, Rubow KL [1983]. An aerosol chamber for instrument evaluation and calibration. *Am Ind Hyg Assoc J* 44(5):361–367.
- Maynard AD, Kenny LC [1995]. Performance assessment of three personal cyclone models, using an aerodynamic particle sizer. *J Aerosol Sci* 26(4):671–684.
- MSHA [2003]. Statement of David D. Lauriski, assistant Secretary of Labor for mine safety and health, before the subcommittee on labor, health and human services, and education, committee on appropriations, United States Senate, July 31, 2003, p. 3. [<http://www.msha.gov/media/congress/2003/07312003.pdf>]. Date accessed: May 2006.
- MSHA [2005]. MSHA standardized information system (Teradata), coal dust data. Date accessed: December 5, 2005. Arlington, VA: U.S. Department of Labor, Mine Safety and Health Administration.

Patashnick H, Rupprecht EG [1991]. Continuous PM-10 measurements using the tapered-element oscillating microbalance. *J Air Waste Manag Assoc* 41(8):1079–1083.

Peters TM, Volkwein JC [2003]. Analysis of sampling line bias on respirable mass measurement. *Appl Occup Environ Hyg* 18(6):458–465.

Rubow KL, Marple VA, Olin J, McCawley MA [1987]. A personal cascade impactor: design, evaluation and calibration. *Am Ind Hyg Assoc J* 48(6):532–538.

Rupprecht and Patashnick Co. [2004]. Operating manual, TEOM series 3700/3700 personal dust monitor, revision A, September 2004, R&P part number 42–009904. Albany, NY: Rupprecht and Patashnick Co., Inc.

Soderholm SC [1989]. Proposed international conventions for particle size-selective sampling. *Ann Occup Hyg* 33(3):301–320.

U.S. Department of Labor [1996]. Report of the Secretary of Labor's advisory committee on the elimination of pneumoconiosis among coal mine workers. Recommendation Nos. 8 and 17. Arlington, VA: U.S. Department of Labor, Mine Safety and Health Administration.

Volkwein JC, Thimons, ED [2001]. New tools to monitor personal exposure to respirable coal mine dust. In: *Proceedings of the Seventh International Mine Ventilation Congress* (Krakow, Poland, June 17–21, 2001), pp. 143–150.

Volkwein JC, Vinson RP, McWilliams LJ, Tuchman DP, Mischler SE [2004]. Performance of a new personal respirable dust monitor for mine use. Pittsburgh, PA: U.S. Department of Health and Human Services, Public Health Service, Centers for Disease Control and Prevention, National Institute for Occupational Safety and Health, DHHS (NIOSH) Publication No. 2004–151, RI 9663.

Williams KL, Timko RJ [1984]. Performance evaluation of a real-time aerosol monitor. Pittsburgh, PA, U.S. Department of the Interior, Bureau of Mines, IC 8968. NTIS No. PB 84–199710.

Williams KL, Vinson RP [1986]. Evaluation of the TEOM dust monitor. Pittsburgh, PA, U.S. Department of the Interior, Bureau of Mines, IC 9119. NTIS No. PB 87–182978.

## Appendix A. Detailed mine PDM concentration data .

MSHA District	Date	Notes Occupation MSHA code	Shearer 64	Mechanic 4	Shearer 64	Shift foreman 49	Faceman 41	Faceman 41	Faceman 41	Faceman 41	Mechanic 4	Headgate 40	Dust sampler 414
9	2-Nov			2.51	1.87	1.37	0.73	0.62	1.72	1.68			
	3-Nov		2.03	1.81	2.17	0.61	2.24	2.8		2.73		1.62	
	4-Nov		0.87	1.75	0.47	0.57	1.32	1.24	0.976	1.74	1.48		
	5-Nov	no prod.	0.44	0.28			0.59		0.37	0.57		0.32	0.23
	6-Nov	no prod.	0.25		0.12			0.17		0.15		0.17	
	7-Nov	no prod.	0.82				0.99	0.66				0.86	
	8-Nov		0.92	0.48	0.8		0.91	1.35	0.77				
	9-Nov			1.6	2.35		3.35	3.41	3.19	3.13			
	10-Nov		2.42				2.68						
	11-Nov				0.91		1.52	1.37	1.47				

	Occupation MSHA code	Miner operator 36	Tube side bolter 48	Intake side bolter 19	Loader operator 43	Standard shuttle car 50	Off std. shuttle car 73	Mechanic 4	Foreman 430	Center bolter 46	Center bolt helper 47
3	14-Dec	0.38	0.69	0.31	1.09	0.26	0.37	0.35	0.5	0.35	0.33
	15-Dec	0.55	0.49	0.54	0.41	0.28	0.33	0.32	0.93	0.6	0.46
	16-Dec	0.48	0.72	0.45	0.37	0.26	0.31	0.4		0.45	0.54
	17-Dec		0.37	0.31	0.35	0.35	0.33	0.36	0.4	0.92	
	20-Dec	0.69		0.57	0.44	0.33	0.36	0.4	0.48	0.07	
	21-Dec		0.32	0.39	0.27	0.24	0.3	0.19	0.72	0.87	
	22-Dec	0.31	0.41	0.4	0.24	0.24	0.19	0.23	0.66	note	

note=cyclone broken but ran in office

	Occupation MSHA code	Shearer Head Operator 064	Shearer Tail Operator 040	Mechanic 1 004	Mechanic 2 004	Jack Setter 1 041	Jack Setter 2 041	Utility 053	Foreman 049
4	4-Jan	0.84	0.66	0.66	0.55	0.97	0.72	0.7	0.79
	5-Jan	1.41	1.07		0.69	1.4	1.29	1.3	
	6-Jan	1.52	1.53	0.57	0.8	1.58	1.69	1.07	1.2
	7-Jan	1.4	0.64	0.56	0.66	1.43	1.33	1.13	1.71
	10-Jan	1.47	1.53	1.36	0.85	1.54	1.51	1.27	1.63
	11-Jan	1.86	1.84	0.25	1.02	2.07	1.56	1.42	1.88
	12-Jan	0.85	0.75	0.59	0.13	1.01	0.97	0.96	0.77
	13-Jan	1.45	1.44	1.05	0.85	1.21	1.24	1.07	1.56

	Occupation MSHA code	Miner Operator 36	Miner helper 35	Intake side bolter 12	Return side bolter 14	Ram Car 2 50	Ram Car 3 50	Ram Car 4 50	Foreman 49	Scoop 54	Curtain 8	Bratticeman 32
11	25-Jan	0.73	0.85	0.9	1.26	0.57	0.46	0.58	0.86	0.92	1.09	
	26-Jan		1.23	0.65	0.9	1.17	0.98	1.16	1.23	0.67	0.58	0.66
	27-Jan	0.61	0.67	1.5	1.31	0.64	0.67	0.61	1.01	0.88	1.67	0.6
	28-Jan	0.58	0.95	0.51	0.43	0.7	0.6	0.58	0.39	0.7	0.41	0.64
	31-Jan	0.53	0.64	0.78	0.79	0.89	0.92	0.96	0.59	0.65	1.01	
	1-Feb	0.5	0.78	1.06	1.05	0.32	0.27	0.36	0.66	0.45		0.36
	2-Feb	0.63	1.16	1.22	1.4	1.13	1.01		0.96		1.53	
	3-Feb	0.77	1.35	2.63	1.65	1.05	0.69	0.86	0.51	1	1.28	

	Occupation MSHA code	Guest	Beltman	Utility	Motorman
11 (Contd)	25-Jan	0.88		0.84	
	26-Jan				
	27-Jan	0.48			
	28-Jan			0.46	
	31-Jan		0.33		
	1-Feb				
	2-Feb				0.57
	3-Feb				

This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.



## Appendix A. Detailed mine PDM concentration data .

		Occupation	Standard shuttle car	Center bolter	Left Return side bolter	Off standard shuttle car	Outby utilityman	Center bolter helper	Mechanic	Miner Operator	Foreman	Load Mach. Oper.	R. intake side bolter	Tubeman brattice
		MSHA code	50	46	14	73	53	47	4	36	49	43	12	32
2	8-Feb		0.23	0.21	0.67	0.38	0.42	0.19		0.50	0.25	0.27	0.65	
	9-Feb		0.14	0.19	0.55	0.21	0.19	0.17	0.19	0.41	0.31	0.18	1.74	0.86
	10-Feb		0.42	0.4	0.78	0.25	0.48	0.24	0.31	0.42	0.31	0.18	0.89	0.73
	11-Feb		0.18	0.25		0.23	0.29	0.41	0.30	0.40	0.45	0.27	0.51	0.64
	14-Feb		0.22	0.20	0.79	0.16		0.24	0.21	0.43	0.29	0.22	0.66	0.55
	15-Feb		0.15	0.24	1.63	0.29		0.21	0.19	0.38	0.52		0.87	0.58
	16-Feb		0.24	0.26	0.82	0.42	0.04	0.26	0.34	0.39	0.42	0.63	0.93	0.96
	17-Feb		0.17	0.18	1.06	0.28		0.32		0.54	0.51	0.41	0.79	1.17
		Occupation	Right Miner operator	Left Miner operator	R. bolt opposite oper.	Right bolter operator	L. bolter opposite op.	Left bolter operator	Shuttle car 1	Shuttle car 2	Shuttle car 3	Shuttle car 4	Foreman	Mechanic
		MSHA code	36	36	12	14	12	14	50	50	50	50	49	4
10	1-Mar		0.86	1.63	0.76	0.55	1.33	1.76	0.82	0.74	0.66	0.63	0.6	0.59
	2-Mar		1.12	1.23	1.1	0.98	1.34	0.99	0.75	0.75	0.72	0.67	0.69	0.57
	3-Mar		1.07	1.73	1.71	0.6	2.48	2.46	0.77	0.83	0.7	0.67	0.56	
	4-Mar		0.68	1.58	0.62	0.6	1.57	2.45*	0.85	0.97	0.79	0.86	0.52	1.35
	5-Mar		0.31	1.62	0.59	1.29	1.5	1.32	0.68	0.8		0.76	1.04	
	7-Mar			1.31	0.32	1.08		2.09	0.77	0.78	0.77	0.66	0.62	0.88
	8-Mar			1.64	0.73	0.92		1.32	0.74	0.89		0.8	0.78	0.89
	9-Mar		1.96	1.96	0.84	1		1.55	1.03	1.08	0.95	0.87	0.7	1.08
	10-Mar		0.67	1.64	0.7	12.12*		6.32*	0.75		0.76		0.53	1.11
*Data valid, voided for cause														
		Occupation	R Bolter op	L Miner operator	SC	Electrician	L Bolter op	R miner operator	SC	Foreman	L Bolter	SC	R miner operator	
		MSHA code	12	36	50	2	14	36	50	49	12	50	36	
6	15-Mar		1.57	1.53	0.66	0.29	1.9	1.08	0.26	0.82	2	0.23		
	16-Mar		1.22	1.7	0.9	1.47	1.65		0.56	1.75	1.7	0.52	0.98	
	17-Mar		1.14	1.6		0.52	1.68		0.34	0.71		0.33	1.16	
		Occupation	#1 Bridge	Left Bolter/right side	Mechanic	#2 Bridge	Right bolter/left side	MSHA	Scoop	R. bolter/r. side	#3 Bridge	Foreman	L. Bolter/l. side	Miner operator
		MSHA code	na	na	na	na	na	na	na	na	na	na	na	na
5	29-Mar		1.42	1.25	0.63	0.58	1.19	1.31	ns	1.02	1.38	0.85	1.04	5.84
	30-Mar		0.34	1.62	1.48	0.87	3.43	ns	3.52	3.01	1.61	2.18	1.26	1.63
	31-Mar		0.32	0.72		0.5	1.17	ns	1.34	0.98	0.7	1.01	0.54	0.84
		Occupation	R Miner operator	L Miner operator	R Intake side bolter	R Return side bolter	L Intake side bolter	L Return side bolter	Coal Hauler 67	Coal Hauler 69	Foreman	Utility	Mechanic	Mechanic
		MSHA code	36	36	12	14	12	14	50	50	49	53	4	4
8	19-Apr		ns		1.61		0.95	2.92	1.64	1.6	1	1.19	1.37	1.05
	20-Apr		ns	1.46	1.75	2.72	1.58	2.52	1.08	1.09	1.68	0.96	0.5	0.54
	21-Apr		0.42	4.24	2.19	3.34	1.15	2.84	1.74	1.74	1.46	1.08	0.74	0.83
		Occupation	Safety	Coal Hauler 66										
		MSHA code		50										
8 (Contd)	19-Apr		0.72	1.6										
	20-Apr		0.69	1.27										
	21-Apr		ns	ns										
		Occupation	Miner operator	Pinner operator	Std shuttle car	Offstd shuttle car	Electrician	Scoop	Foreman	NIOSH 1	NIOSH 2	MSHA		
		MSHA code	36	12	50	73	2	54	49					
7	17-May		0.35	0.24	0.29	0.24	0.34	0.23	0.17	0.47				
	18-May		1.27	0.32	0.3		0.58		0.25	0.29	0.963	0.7		
	19-May		1.01	0.6	0.26		0.28	2.67	0.27					

na= not available

This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.

## Appendix B Detailed mine Lippmann sampler data.

MSHA			PDM					Dorr-Oliver 2 L/min						MRE Equiv	Dorr-Oliver 1.7 L/min					SIZE DISTRIBUTIONS			
			Dist.	Date	PDM #	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>	std mg/m <sup>3</sup>	RSD	mass mg	time min	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>		std mg/m <sup>3</sup>	RSD	conc mg/m <sup>3</sup>	mass mg	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>	std mg/m <sup>3</sup>	RSD	Inst #
20 mile	9	2-Nov	102	1.367				0.731		1.030					0.753	1.248					1	9.38	2.65
			122	1.475	1.397	0.068	0.049	0.750	355	1.056	1.046	0.014	0.013	1.443	0.711	1.178	1.228	0.044	0.036		2	9.35	2.51
			108	1.349				0.746		1.051					0.760	1.259				3	8.85	3.00	
	9	3-Nov	102	1.630				0.787		1.234					0.788	1.453					4	10.00	2.99
			122	1.771	1.662	0.097	0.058	0.788	319	1.235	1.204	0.052	0.043	1.662	0.777	1.433	1.432	0.021	0.015		5	7.13	2.58
			108	1.586				0.730		1.144					0.765	1.411				6	8.27	2.59	
	9	4-Nov	102	1.239				0.645		0.849					0.658	1.019					7	8.67	2.84
			122	1.307	1.215	0.106	0.087	0.664	380	0.874	0.842	0.036	0.043	1.161	0.667	1.033	1.010	0.027	0.027		8	7.48	2.57
			108	1.099				0.610		0.803					0.633	0.980				9	7.43	2.74	
Blacksville	3	14-Dec	115	0.365				0.059		0.271					0.062	0.335					7	8.68	2.34
			130	0.363	0.358	0.012	0.033	0.053	109	0.243	0.245	0.025	0.103	0.338	0.058	0.313	0.309	0.027	0.088		8	8.17	2.89
			135	0.344				0.048		0.220					0.052	0.281				9	8.19	3.06	
	3	15-Dec	115	1.506				0.614		1.023					0.679	1.331					10	6.56	2.59
			130	1.602	1.479	0.137	0.093	PF	300		1.045	0.031	0.029	1.442	0.636	1.247	1.252	0.077	0.061		11	7.32	2.90
			135	1.331				0.640		1.067					0.601	1.178				14	7.26	2.39	
	3	16-Dec	115	0.755				0.331		0.522					0.319	0.592					16	7.08	2.58
			130	0.826	0.764	0.058	0.076	0.342	317	0.539	0.515	0.029	0.057	0.710	0.314	0.583	0.622	0.060	0.096		17	7.53	2.57
			135	0.711				0.306		0.483					0.372	0.690				19	7.54	2.44	
Harris	4	4-Jan	115	2.655				0.954		2.129					0.866	2.273					1	5.49	2.83
			120	2.472	2.549	0.095	0.037	0.906	224	2.022	2.087	0.057	0.028	2.880	0.851	2.234	2.302	0.086	0.038		2	6.11	3.13
			135	2.519				0.946		2.111					0.914	2.399				3	5.34	3.02	
	4	5-Jan	115	1.988				0.447		1.519					0.413	1.651					4	6.06	2.92
			120	2.151	2.051	0.088	0.043	0.444	147	1.509	1.481	0.058	0.039	2.043	0.413	1.651	1.687	0.062	0.037		5	6.13	2.87
			135	2.013				0.416		1.414					0.440	1.759				6	5.92	2.90	
	4	6-Jan	115	1.812				0.517		1.520					0.451	1.559					7	5.96	2.90
			120	1.887	1.868	0.049	0.026	0.498	170	1.464	1.457	0.066	0.046	2.010	0.481	1.663	1.629	0.060	0.037		8	7.17	2.66
			135	1.905				0.472		1.387					0.481	1.663				25	6.24	3.27	
P&M	11	25-Jan	115	2.129				0.745		1.816					0.699	2.005					1	7.10	3.21
			120	2.147	2.228	0.156	0.070	0.735	205	1.792	1.774	0.054	0.030	2.448	0.692	1.985	2.023	0.050	0.025		2	6.93	3.23
			127	2.407				0.703		1.714					0.725	2.079				3	6.03	3.18	
	11	26-Jan	115	0.609				0.267		0.474					0.256	0.535					4	10.09	3.87
			120	0.599	0.626	0.038	0.061	0.264	281	0.469	0.461	0.019	0.042	0.636	0.262	0.548	0.546	0.011	0.019		5	9.21	3.23
			127	0.670				0.247		0.439					0.266	0.556				6	9.15	3.47	
	11	27-Jan	115	1.732				0.761		1.435					0.700	1.553					7	6.67	3.29
			120	1.794	1.760	0.031	0.018	0.771	265	1.454	1.418	0.047	0.033	1.957	0.700	1.553	1.558	0.009	0.006		8	6.21	3.48
			127	1.754				0.724		1.365					0.707	1.569				25	6.08	3.32	
Emerald	2	8-Feb	115	0.750				0.156		0.630					0.138	0.656					16	8.19	2.61
			120	FL	0.827	0.109	0.132	0.142	124	0.574	0.594	0.031	0.053	0.820	0.141	0.670	0.685	0.038	0.055		17	10.89	2.82
			127	0.904				0.143		0.578					0.153	0.727				18	10.68	2.44	
	2	9-Feb	115	2.310				0.735		1.802					0.681	1.965					19	7.23	2.68
			120	2.300	2.373	0.118	0.050	0.749	204	1.837	1.779	0.073	0.041	2.454	0.708	2.042	2.017	0.045	0.022		20	7.25	2.89
			127	2.510				0.692		1.697					0.708	2.042				21	6.91	2.78	
	2	10-Feb	115	0.660				0.213		0.539					0.204	0.607					22	11.44	3.20
			120	NF	0.710	0.071	0.100	0.217	198	0.549	0.529	0.027	0.051	0.729	0.213	0.634	0.631	0.022	0.036		23	13.15	3.16
			127	0.760				0.197		0.498					0.219	0.652				24	11.60	3.34	

PF Pump failure

NF Filter not installed

FL PDM file data was a constant value.

This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.

## Appendix B Detailed mine Lippmann sampler data.

MSHA			PDM					Dorr-Oliver 2 L/min						MRE Equiv	Dorr-Oliver 1.7 L/min					SIZE DISTRIBUTIONS		
Dist.	Date		PDM #	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>	std mg/m <sup>3</sup>	RSD	mass mg	time min	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>	std mg/m <sup>3</sup>	RSD	conc mg/m <sup>3</sup>	mass mg	conc mg/m <sup>3</sup>	ave mg/m <sup>3</sup>	std mg/m <sup>3</sup>	RSD	Inst #	MMD	GSD
Freedom	10	1-Mar	115	1.839				0.518		1.727					0.461	1.808				7	7.33	3.08
			124	1.879	1.861	0.020	0.011	0.486	150	1.620	1.659	0.059	0.036	2.289	0.476	1.867	1.841	0.030	0.016	8	9.02	3.62
			127	1.865				0.489		1.630					0.471	1.847				9	6.82	3.08
	10	2-Mar	115	1.255				0.554		1.045					0.269	0.597				10	5.44	2.84
			124	1.322	1.308	0.048	0.036	0.559	265	1.055	1.045	0.010	0.010	1.442	0.545	1.210	0.995	0.345	0.347	11	5.75	2.87
			127	1.347				0.548		1.034					0.531	1.179				12	5.40	2.97
	10	3-Mar	115	1.749				0.768		1.542					0.708	1.673				13	5.56	3.29
			124	1.770	1.800	0.072	0.040	0.768	249	1.542	1.524	0.031	0.021	2.103	0.735	1.736	1.693	0.038	0.022	14	6.02	3.26
			127	1.882				0.741		1.488					0.707	1.670				15	5.35	3.20
Johns Ck	6	15-Mar	115	2.550				1.094		2.223					1.037	2.479				1	6.52	2.90
			124	2.704	2.683	0.124	0.046	1.040	246	2.113	2.162	0.056	0.026	2.983	0.988	2.362	2.445	0.072	0.030	2	6.27	3.01
			127	2.796				1.058		2.150					1.043	2.493				3	6.93	2.95
	6	16-Mar	115	3.955				0.874		3.610					0.815	3.960				4	5.14	3.74
			124	4.181	3.494	1.000	0.286	0.812	121	3.354	3.504	0.134	0.038	4.836	0.784	3.810	3.857	0.090	0.023	5	5.94	3.56
			127	2.347				0.859		3.548					0.782	3.800				6	6.37	3.46
	6	17-Mar	115	4.400				1.072		4.219					0.953	4.413				7	7.44	3.02
			124	4.534	4.631	0.292	0.063	0.982	127	3.865	4.009	0.186	0.046	5.533	0.967	4.477	4.476	0.063	0.014	8	9.85	3.46
			127	4.960				1.002		3.944					0.980	4.538				9	8.86	3.17
Fork Ridge	5	29-Mar	124	12.149				1.128		9.400					1.171	11.480				1	5.80	2.86
			127	13.241	12.370	0.785	0.063	1.141	60	9.508	9.578	0.221	0.023	13.217	1.125	11.029	11.261	0.226	0.020	18	5.66	2.67
			130	11.719				1.179		9.825					1.150	11.275				19	5.89	2.97
	5	30-Mar	124	3.633				0.810		3.045					0.759	3.357				20	4.12	2.66
			127	3.741	3.668	0.064	0.017	0.595	133	2.237	2.774	0.466	0.168	3.829	0.761	3.366	3.351	0.018	0.005	21	4.24	2.80
			130	3.629				0.809		3.041					0.753	3.330				22	4.19	2.95
	5	31-Mar	124	2.165				0.753		1.651					0.703	1.814				23	4.03	3.03
			127	2.287	2.184	0.094	0.043	0.804	228	1.763	1.722	0.062	0.036	2.377	0.632	1.631	1.786	0.144	0.081	24	4.40	3.15
			130	2.101				0.799		1.752					0.742	1.914				25	3.97	2.68
Air Quality	8	19-Apr	111	3.332				1.312		3.066					1.164	3.200				1	4.04	4.86
			114	3.188	3.241	0.079	0.024	1.246	214	2.912	3.012	0.087	0.029	4.157	1.149	3.159	3.179	0.021	0.006	2	3.71	4.63
			126	3.203				1.309		3.059					1.156	3.178				3	3.52	4.75
	8	20-Apr	111	4.549				1.114		4.253					0.949	4.263				4	3.89	3.90
			114	4.492	4.495	0.053	0.012	1.100	131	4.200	4.210	0.039	0.009	5.810	0.991	4.451	4.276	0.169	0.039	5	4.14	3.70
			126	4.443				1.094		4.177					0.916	4.115				6	3.56	3.49
	8	21-Apr	111	6.881				1.274		6.372					1.075	6.325				7	4.55	3.52
			114	6.779	6.748	0.151	0.022	1.218	100	6.092	6.095	0.275	0.045	8.411	1.124	6.614	6.525	0.174	0.027	8	3.95	3.46
			126	6.584				1.164		5.822					1.128	6.637				9	3.90	3.63
Panther	7	17-May	111	4.269				1.122		3.320					1.138	3.961				7	4.32	2.47
			114	4.218	4.274	0.058	0.014	1.151	169	3.405	3.409	0.092	0.027	4.705	1.129	3.930	3.909	0.065	0.017	8	4.36	2.86
			126	4.334				1.184		3.503					1.102	3.836				9		
	7	18-May	111	6.529				1.399		5.032					1.437	6.081				10	4.35	2.89
			114	6.342	6.425	0.095	0.015	1.437	139	5.169	5.199	0.184	0.035	7.175	1.344	5.688	5.863	0.200	0.034	11	4.27	2.91
			126	6.405				1.500		5.396					1.375	5.819				12	4.52	2.29
	7	19-May	111	2.594				0.741		2.047					0.709	2.304				13	5.91	3.02
			114	2.566	2.565	0.029	0.011	0.719	181	1.986	2.044	0.057	0.028	2.821	0.699	2.272	2.277	0.025	0.011	14		
			126	2.536				0.760		2.099					0.694	2.255				15	6.25	2.38

This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.

## APPENDIX C.—ANALYSIS OF VOIDED RESPIRABLE COAL MINE DUST SAMPLES COLLECTED, 1995–2004

The causes for void samples in Table C–1 below include factors in addition to mechanical faults of the samplers. Samples collected by both inspectors and coal mine operators are listed. Use of the PDM may significantly reduce the number of samples voided for a number of different causes. The types of causes amenable to prevention by the PDM are those that relate to documentation, timing, and (in the case of some) sample weight issues. The PDM generates a unique data file for each sample that includes the date, time, and various instrument operating parameters, eliminating many documentation issues. The PDM is also programmable to start and stop at specific times, avoiding excess sample times. In addition, the PDM provides EOS mass and concentration values, eliminating shipping, holding, and some laboratory issues. Causes that are considered amenable to reduction by the PDM are indicated by a footnote in the table below. Note that certain codes apply only to either inspector or operator samples.

**Table C–1.—Analysis of voided respirable coal mine dust samples collected, 1995–2004**

	Inspector samples	Operator samples
Total samples collected .....	381,335	487,713
Nonvoided samples .....	357,936 (93.9%)	430,710 (88.3%)
Voided samples .....	23,399 (6.1%)	57,003 (11.7%)
<b>BREAKDOWN OF VOIDED SAMPLES</b>		
Abnormal tamper-resistant .....	NA	14
Abnormal white center .....	NA	6
Broken <sup>1</sup> .....	204	1,452
Cassette did not match card <sup>1</sup> .....	63	897
Cassette not received <sup>1</sup> .....	2	45
Contaminated <sup>1</sup> .....	1,166	3,023
Dated before notice <sup>1</sup> .....	NA	1,459
Designated area not in producing status .....	3	2,123
Designated work position not in producing status .....	2	919
Discarded sample (too old) <sup>1</sup> .....	NA	2,487
Dust data card not received <sup>1</sup> .....	3	5
Excess sample <sup>1</sup> .....	1	17,431
Inspector void; rain .....	264	NA
Insufficient dust observed .....	189	867
Insufficient weight gain .....	27	3,966
Invalid certification number .....	76	610
Invalid initial weight <sup>1</sup> .....	108	320
Invalid occupation code .....	4	NA
Invalid or missing date <sup>1</sup> .....	2	2
Invalid or missing time <sup>1</sup> .....	5,407	4,477
Invalid Part 90 miner ident. ....	NA	1
Invalid production .....	11,359	9,923
Invalid sample type .....	547	1,410
Invalid work position .....	21	1
Invalid work shift .....	2,473	20
Malfunctioning pump <sup>1</sup> .....	1,115	15
Mine not in producing status .....	2	NA
Mining machine unit not in producing status .....	NA	1,101
Nonapproved equipment .....	NA	5

<sup>1</sup> Amenable to prevention by the PDM.

*This information is distributed solely for the purpose of pre-dissemination peer review under applicable information quality guidelines. It has not been formally disseminated by the National Institute for Occupational Safety and Health. It does not represent and should not be construed to represent any agency determination or policy.*

**Table C–1.—Analysis of voided respirable coal mine dust samples collected, 1995–2004—Continued**

BREAKDOWN OF VOIDED SAMPLES—Continued		
Occupation code–meth mining mismatch.....	4	NA
Operator void; equipment.....	10	2,083
Operator void; location.....	2	492
Operator void; miscellaneous.....	36	116
Operator void; production.....	30	470
Operator void; rain.....	6	15
Operator void; time.....	13	385
Oversize particles <sup>1</sup> .....	263	390
Part 90 miner not available.....	NA	8
Predated <sup>1</sup> .....	4	88
Quartz laboratory void.....	7	45
Sample not voided.....	357,936	430,710
Sample received while in hold <sup>1</sup> .....	NA	191
Unacceptable timeframe <sup>1</sup> .....	NA	4
Unauthorized work position.....	6	137
Total.....	381,355	487,713
Voided samples potentially prevented by PDM.....	8,338	32,286
Percent of voided samples potentially prevented by PDM.....	35.6	56.6

NA Not applicable.

<sup>1</sup> Amenable to prevention by the PDM.

Source: MSHA [2005].